

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121816\
 Data File : BF091764.D
 Acq On : 19 Dec 2016 4:52
 Operator : UM/SJ
 Sample : H6011-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-24

Quant Time: Dec 19 06:15:26 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 17 22:53:54 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.76	152	304169	20.00	ng	-0.01
21) Naphthalene-d8	8.05	136	1283285	20.00	ng	-0.01
38) Acenaphthene-d10	9.80	164	626696	20.00	ng	-0.01
63) Phenanthrene-d10	11.29	188	1078829	20.00	ng	0.00
75) Chrysene-d12	13.92	240	839650	20.00	ng	-0.01
86) Perylene-d12	15.32	264	627754	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	1017427	56.04	ng	0.00
7) Phenol-d6	6.41	99	829710	37.47	ng	-0.01
23) Nitrobenzene-d5	7.33	82	1547616	69.55	ng	-0.01
41) 2,4,6-Tribromophenol	10.60	330	693249	130.45	ng	0.00
44) 2-Fluorobiphenyl	9.14	172	2857022	91.59	ng	0.00
78) Terphenyl-d14	12.88	244	2359392	70.95	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121816\
Data File : BF091764.D
Acq On : 19 Dec 2016 4:52
Operator : UM/SJ
Sample : H6011-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-24

Quant Time: Dec 19 06:15:26 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 22:53:54 2016
Response via : Initial Calibration

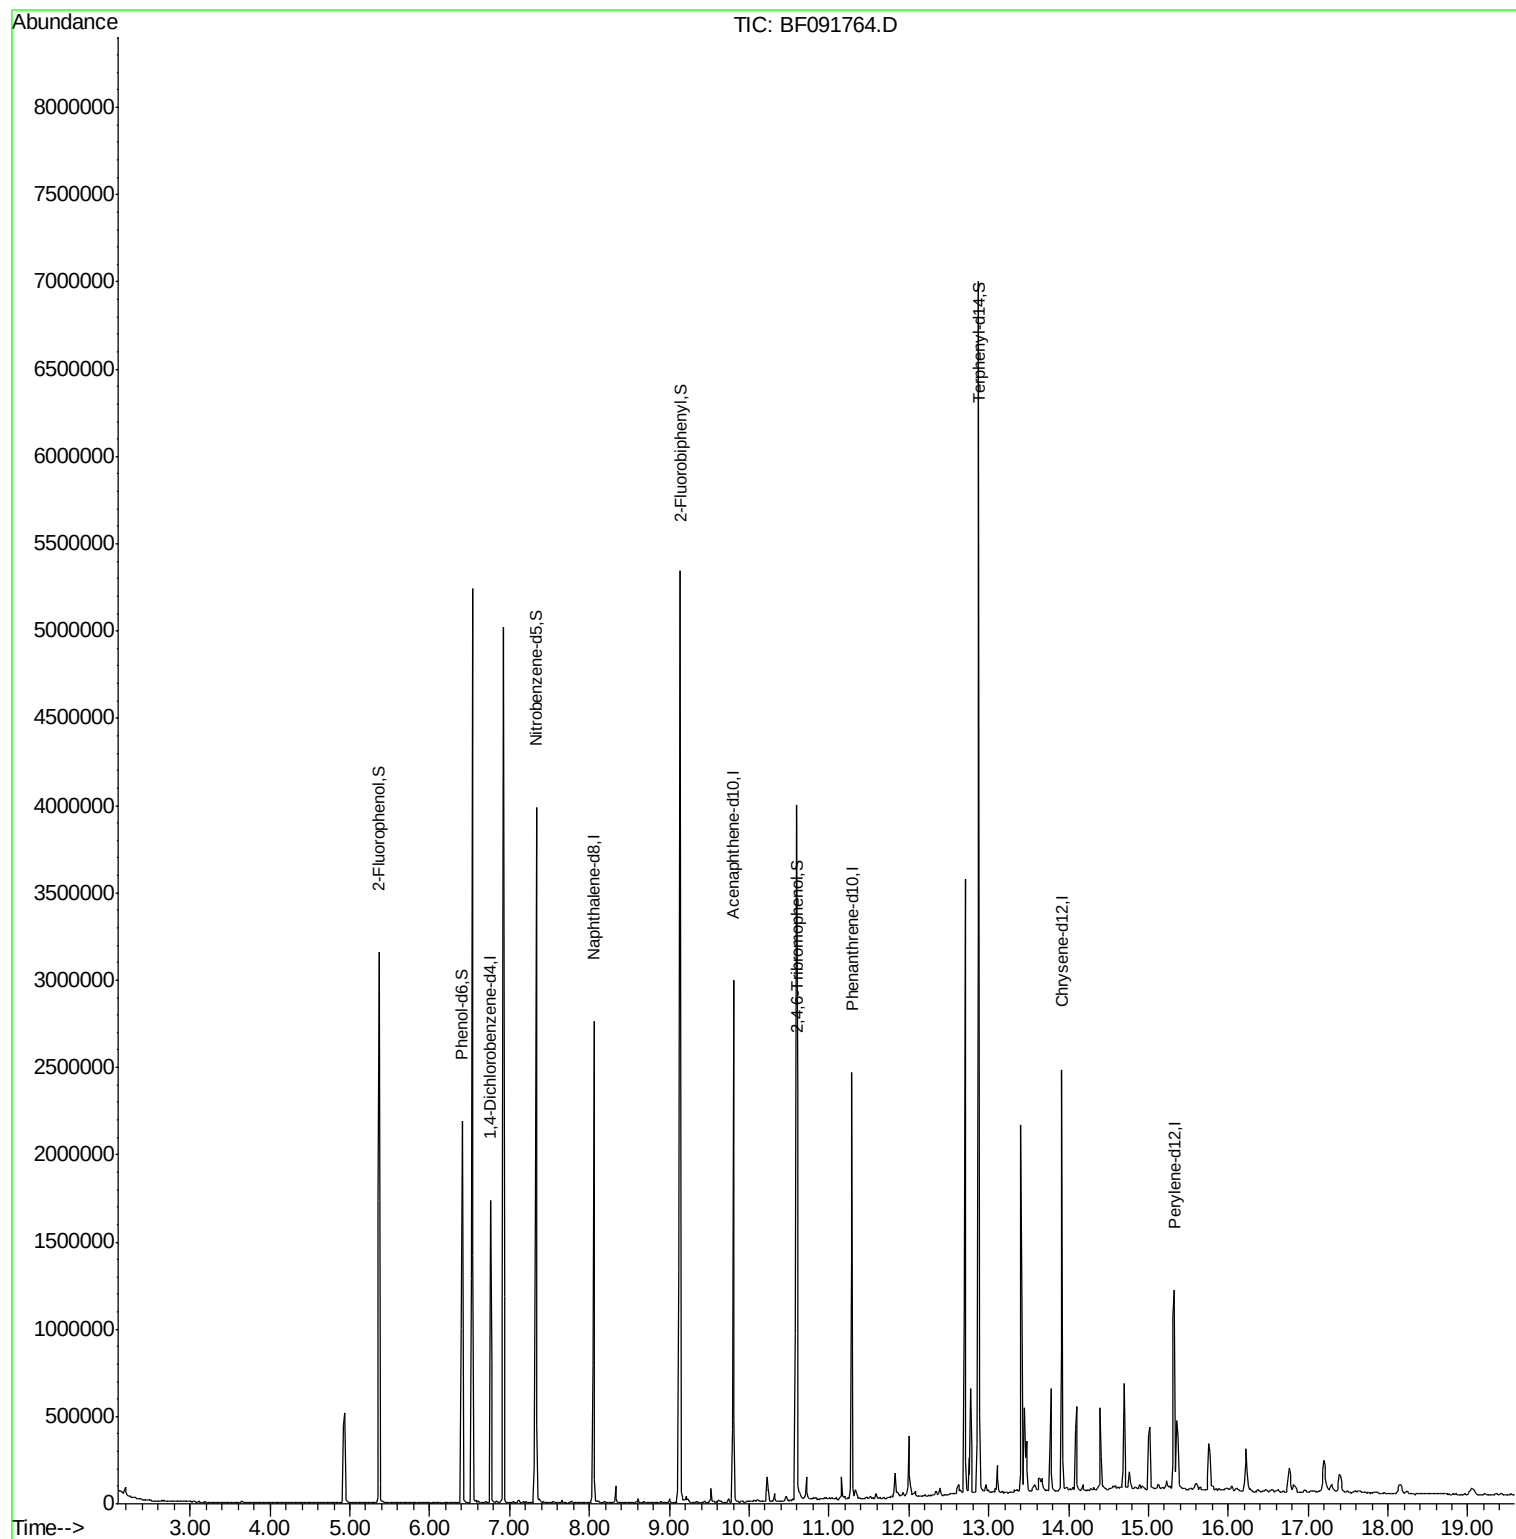

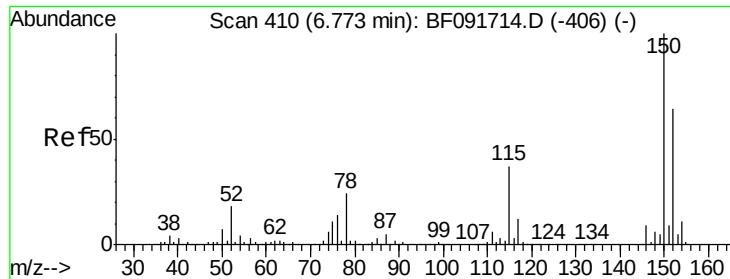

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.76 min Scan# 409

Delta R.T. -0.01 min

Lab File: BF091764.D

Acq: 19 Dec 2016 4:52

Instrument :

BNA_F

ClientSampleId :

MW-24


Tot Ion:152 Resp: 304169

Ion Ratio Lower Upper

152 100

150 158.4 124.9 187.3




115 67.9 46.0 69.0

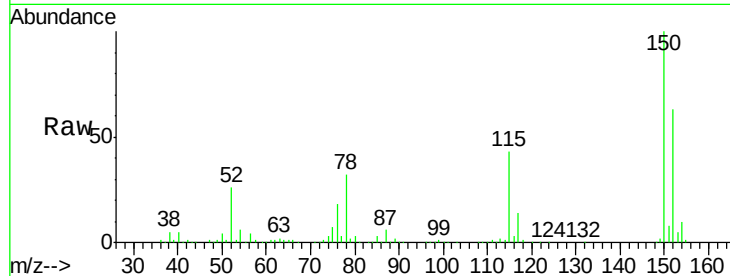

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

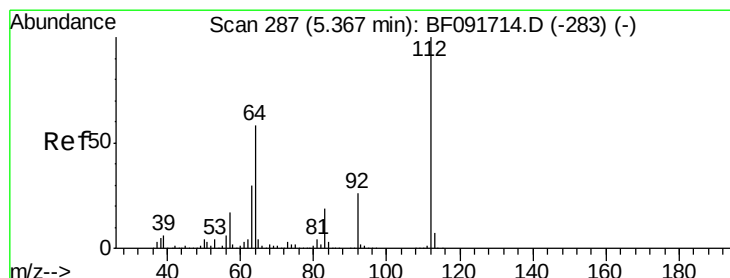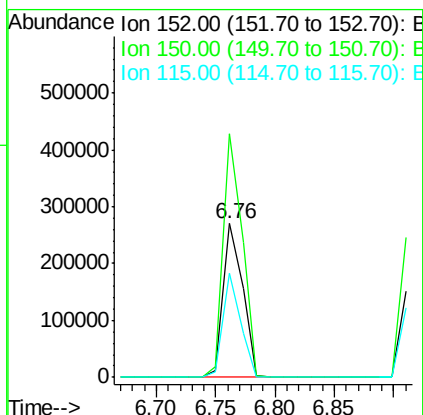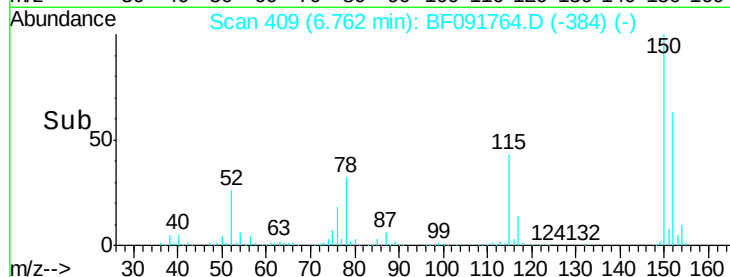

#5

2-Fluorophenol

Concen: 56.04 ng

RT: 5.37 min Scan# 287

Delta R.T. 0.00 min

Lab File: BF091764.D

Acq: 19 Dec 2016 4:52


Tgt Ion:112 Resp: 1017427

Ion Ratio Lower Upper

112 100

64 54.5 46.1 69.1



63 28.0 23.8 35.6

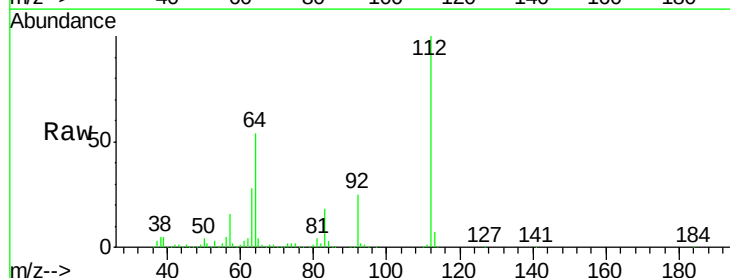


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

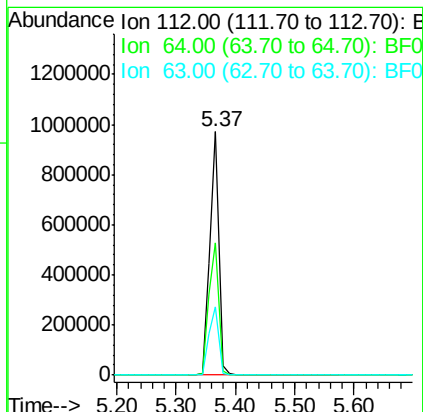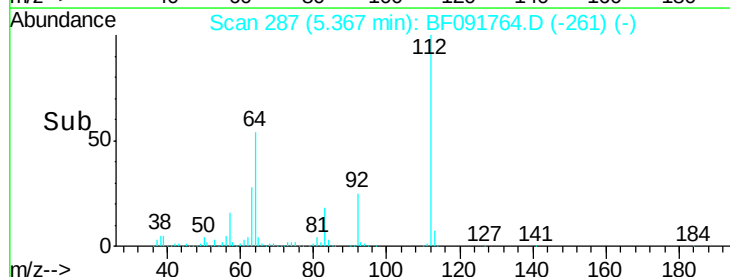

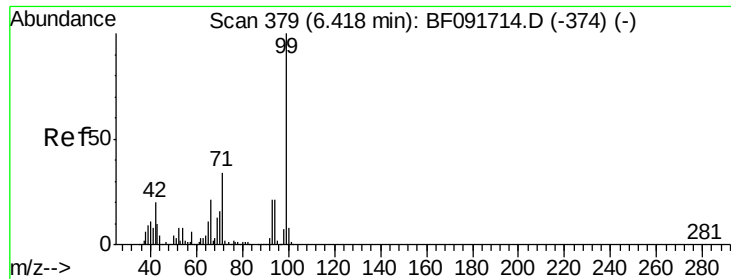

#7

Phenol-d6

Concen: 37.47 ng

RT: 6.41 min Scan# 378

Delta R.T. -0.01 min

Lab File: BF091764.D

Acq: 19 Dec 2016 4:52

Instrument :

BNA_F

ClientSampled :

MW-24


Tot Ion: 99 Resp: 829710

Ion Ratio Lower Upper

99 100

42 15.7 15.6 23.4




71 30.5 27.5 41.3



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

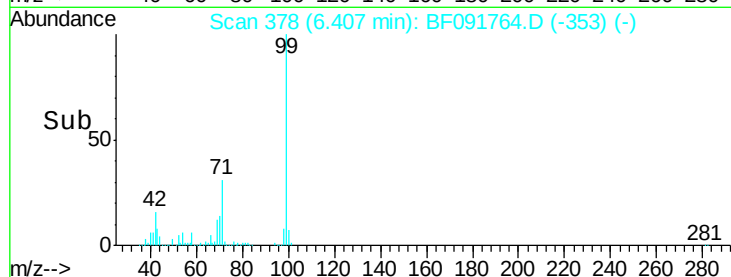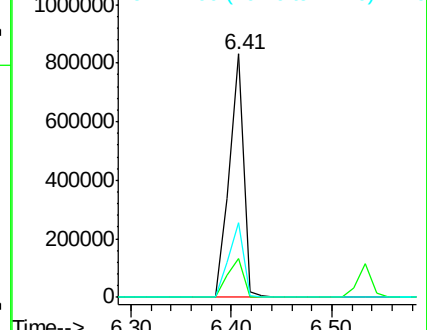

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.05 min Scan# 522

Delta R.T. -0.01 min

Lab File: BF091764.D

Acq: 19 Dec 2016 4:52

Tgt Ion: 136 Resp: 1283285


Ion Ratio Lower Upper

136 100

137 11.4 8.4 12.6

54 7.4 4.5 6.7#

68 5.9 3.6 5.4#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

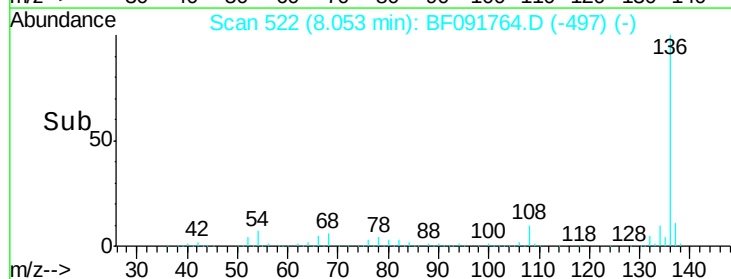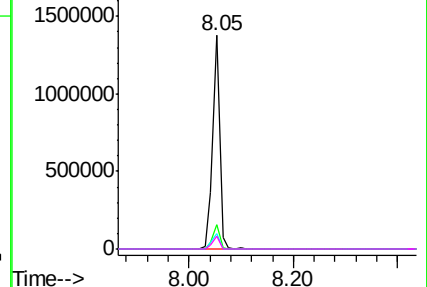


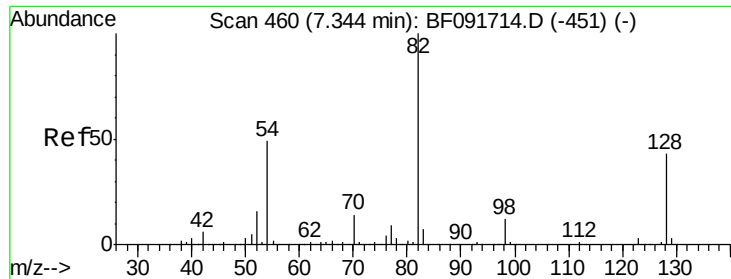




#23
 Nitrobenzene-d5
 Concen: 69.55 ng
 RT: 7.33 min Scan# 459
 Delta R.T. -0.01 min
 Lab File: BF091764.D
 Acq: 19 Dec 2016 4:52

Instrument :
 BNA_F
 ClientSampleId :
 MW-24

Tot Ion: 82 Resp: 1547616
 Ion Ratio Lower Upper
 82 100
 128 41.7 34.6 52.0
 54 50.9 39.5 59.3

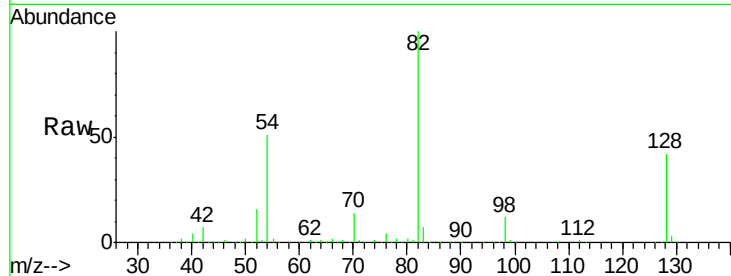


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

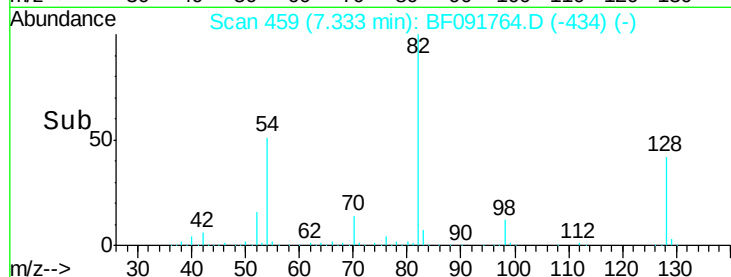
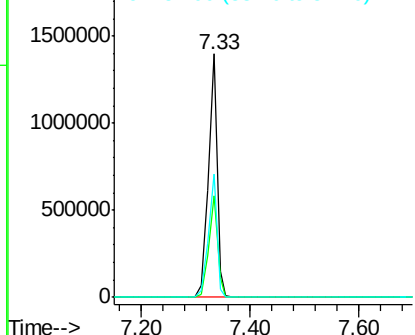



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.80 min Scan# 675
 Delta R.T. -0.01 min
 Lab File: BF091764.D
 Acq: 19 Dec 2016 4:52

Tgt Ion:164 Resp: 626696
 Ion Ratio Lower Upper
 164 100
 162 101.2 80.2 120.2
 160 46.1 36.9 55.3



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



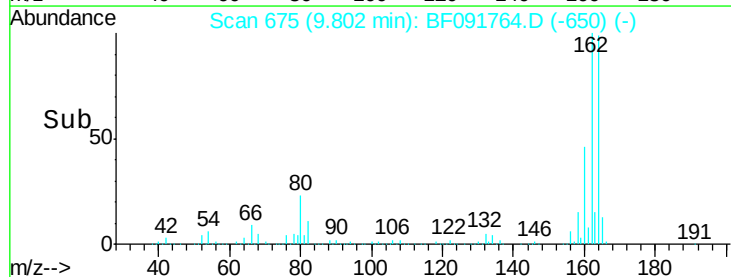
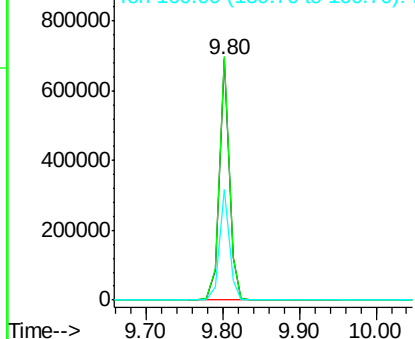


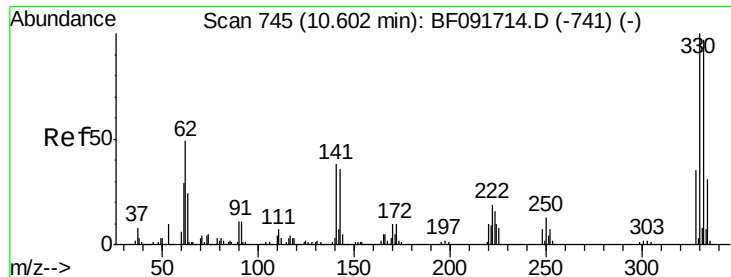

#41
 2,4,6-Tribromophenol
 Concen: 130.45 ng
 RT: 10.60 min Scan# 745
 Delta R.T. 0.00 min
 Lab File: BF091764.D
 Acq: 19 Dec 2016 4:52




Instrument :
 BNA_F
 ClientSampleId :
 MW-24


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.6	77.4	116.2
141	31.5	34.1	51.1#

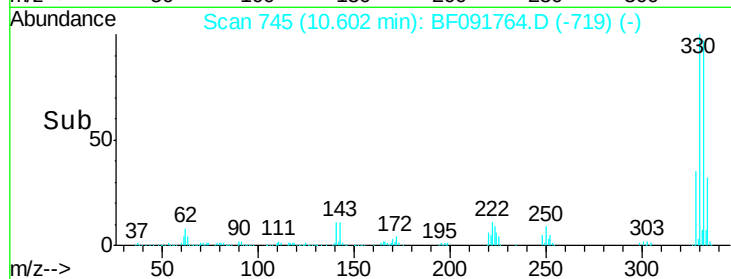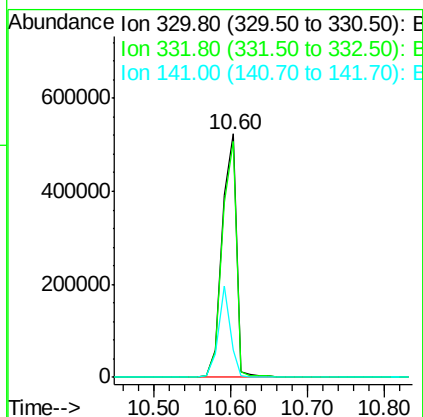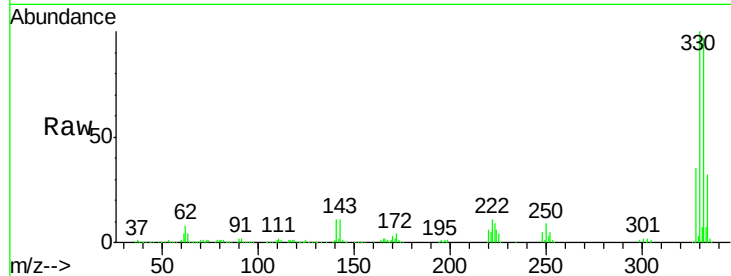

#44
 2-Fluorobiphenyl
 Concen: 91.59 ng
 RT: 9.14 min Scan# 617
 Delta R.T. 0.00 min
 Lab File: BF091764.D
 Acq: 19 Dec 2016 4:52

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	29.4	44.0
170	24.7	20.2	30.4

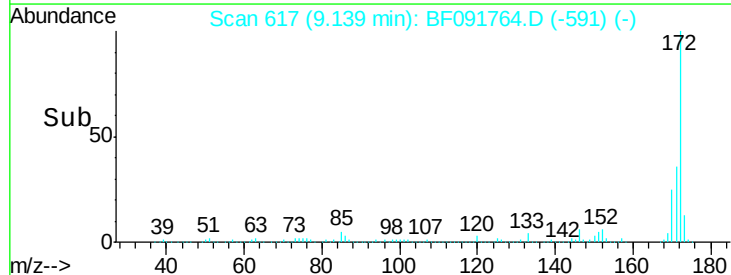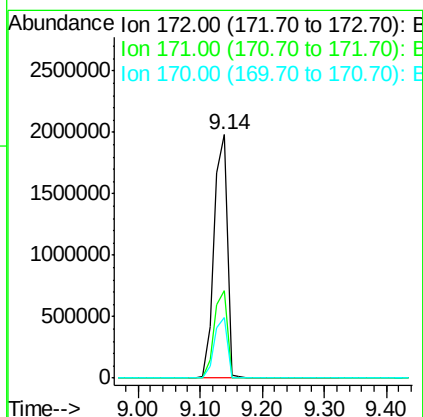


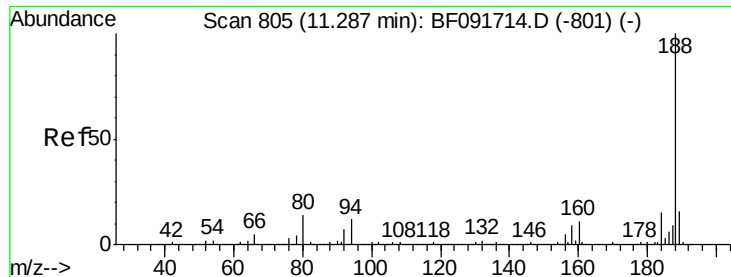




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.29 min Scan# 805
Delta R.T. 0.00 min
Lab File: BF091764.D
Acq: 19 Dec 2016 4:52

Instrument :
BNA_F
ClientSampled :
MW-24

Tot Ion:188 Resp: 1078829
Ion Ratio Lower Upper
188 100
94 7.4 10.0 15.0#
80 7.5 11.2 16.8#

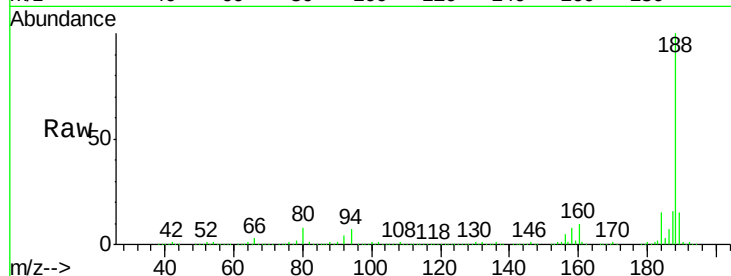


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

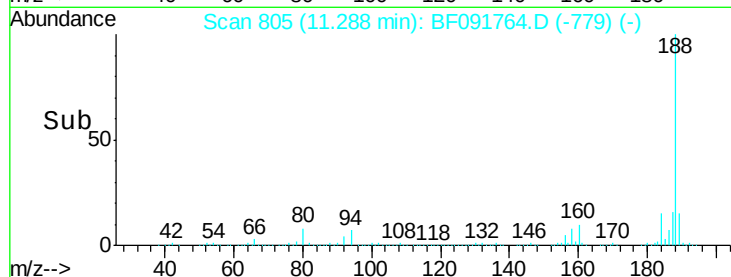
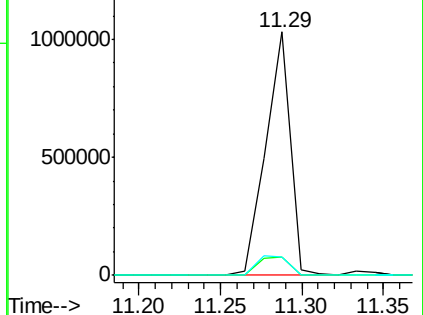



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.92 min Scan# 1035
Delta R.T. -0.01 min
Lab File: BF091764.D
Acq: 19 Dec 2016 4:52

Tgt Ion:240 Resp: 839650
Ion Ratio Lower Upper
240 100
120 10.8 12.9 19.3#
236 26.0 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

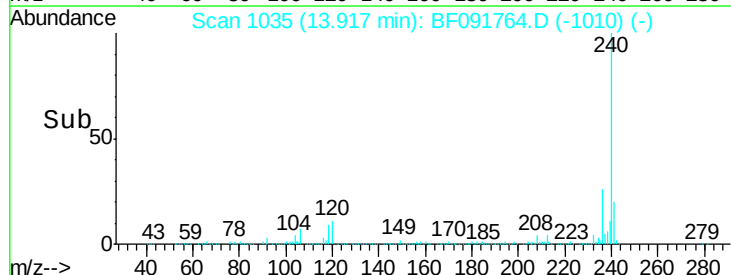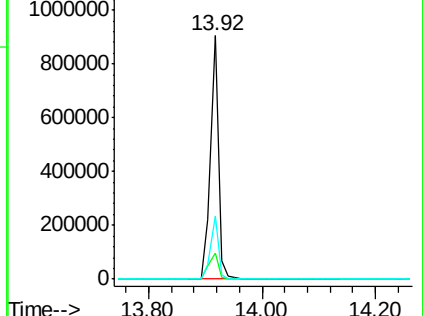


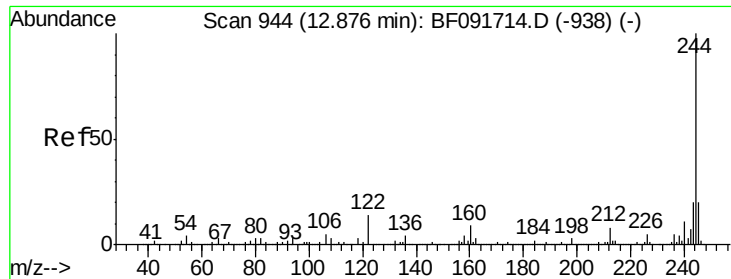




#78
 Terphenyl-d14
 Concen: 70.95 ng
 RT: 12.88 min Scan# 944
 Delta R.T. 0.00 min
 Lab File: BF091764.D
 Acq: 19 Dec 2016 4:52

Instrument :
 BNA_F
 ClientSampleId :
 MW-24

Tot Ion:244 Resp: 2359392
 Ion Ratio Lower Upper
 244 100
 212 7.9 6.2 9.2
 122 13.3 11.4 17.2




Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

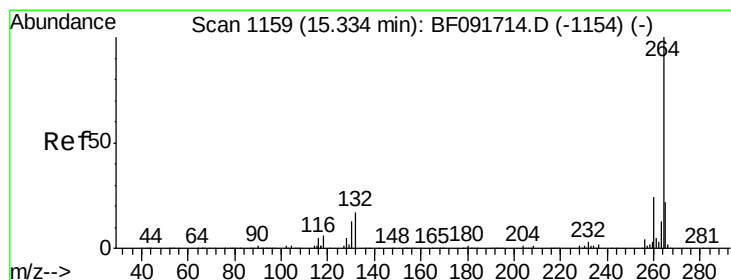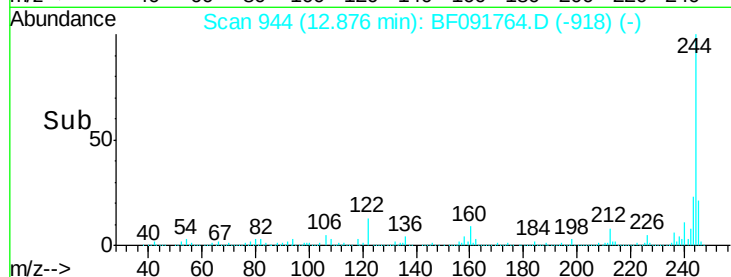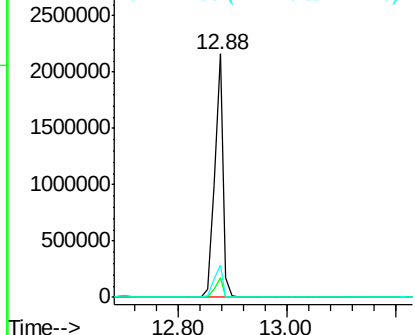

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.32 min Scan# 1158
 Delta R.T. -0.01 min
 Lab File: BF091764.D
 Acq: 19 Dec 2016 4:52

Tgt Ion:264 Resp: 627754
 Ion Ratio Lower Upper
 264 100
 260 24.0 19.2 28.8
 265 21.2 17.4 26.0



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

