

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121816\
 Data File : BF091767.D
 Acq On : 19 Dec 2016 6:14
 Operator : UM/SJ
 Sample : H6006-22DL 5X
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-2-0-5DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.910	245	247	251	rBV	101380	148911	4.83%	0.477%
2	5.356	284	286	289	rBV	367868	358882	11.65%	1.150%
3	6.407	375	378	382	rBV	477516	635929	20.65%	2.038%
4	6.533	387	389	391	rBV	646836	555414	18.03%	1.780%
5	6.762	407	409	412	rBV	1068466	1214269	39.43%	3.892%
6	6.922	420	423	425	rBV	412275	358066	11.63%	1.148%
7	7.322	456	458	461	rBV	246247	335037	10.88%	1.074%
8	8.053	519	522	524	rBV	1944252	1733076	56.27%	5.555%
9	9.128	614	616	618	rBV	1085143	920877	29.90%	2.951%
10	9.528	649	651	653	rVV	118115	109620	3.56%	0.351%
11	9.665	661	663	665	rBV	86696	72121	2.34%	0.231%
12	9.802	673	675	677	rVV	1840916	1668143	54.16%	5.347%
13	9.836	677	678	680	rVB	148791	112305	3.65%	0.360%
14	10.008	691	693	695	rBV	90351	82006	2.66%	0.263%
15	10.351	721	723	725	rVV	117748	113159	3.67%	0.363%
16	10.419	725	729	732	rVV4	12051	35438	1.15%	0.114%
17	10.511	735	737	739	rVB	33869	37627	1.22%	0.121%
18	10.591	741	744	746	rBV	455464	484878	15.74%	1.554%
19	10.716	750	755	759	rBV	66349	91865	2.98%	0.294%
20	10.899	768	771	775	rBV3	23413	50513	1.64%	0.162%
21	11.048	779	784	786	rBV3	29618	65509	2.13%	0.210%
22	11.093	786	788	790	rVB	79278	94259	3.06%	0.302%
23	11.139	790	792	793	rBV	30215	38770	1.26%	0.124%
24	11.185	793	796	799	rVB2	57900	130133	4.23%	0.417%
25	11.288	802	805	806	rBV	1489160	1840741	59.77%	5.900%
26	11.311	806	807	809	rVV	1536158	1103297	35.82%	3.536%
27	11.356	809	811	813	rVB	319850	301628	9.79%	0.967%
28	11.391	813	814	817	rVB	39290	38491	1.25%	0.123%
29	11.516	822	825	827	rBV	191230	217448	7.06%	0.697%
30	11.585	829	831	832	rVV	54753	51052	1.66%	0.164%
31	11.619	832	834	836	rVV2	34094	33435	1.09%	0.107%
32	11.676	837	839	843	rVB4	23055	50613	1.64%	0.162%
33	11.791	846	849	850	rBV	103130	171694	5.57%	0.550%
34	11.813	850	851	853	rVB	248777	187738	6.10%	0.602%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121816\
 Data File : BF091767.D
 Acq On : 19 Dec 2016 6:14
 Operator : UM/SJ
 Sample : H6006-22DL 5X
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-2-0-5DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.859	853	855	856 rBV	80795	71855	2.33%	0.230%
36	11.894	856	858	863 rVB2	246426	362569	11.77%	1.162%
37	11.974	863	865	866 rBV2	23830	47722	1.55%	0.153%
38	11.996	866	867	870 rVV2	42886	47280	1.54%	0.152%
39	12.099	873	876	880 rVB2	131534	250982	8.15%	0.804%
40	12.225	885	887	889 rBV3	28191	47604	1.55%	0.153%
41	12.259	889	890	891 rBV	39708	32342	1.05%	0.104%
42	12.339	894	897	898 rBV	78267	106950	3.47%	0.343%
43	12.385	898	901	902 rBV2	40544	74346	2.41%	0.238%
44	12.419	902	904	906 rVB	131447	142503	4.63%	0.457%
45	12.499	908	911	913 rBV	1539233	1969938	63.96%	6.314%
46	12.556	913	916	917 rBV2	35209	55946	1.82%	0.179%
47	12.591	917	919	920 rVB	63313	63011	2.05%	0.202%
48	12.636	920	923	927 rBV3	49670	132736	4.31%	0.425%
49	12.716	927	930	933 rBV2	1323764	1808538	58.72%	5.797%
50	12.774	933	935	939 rVB2	70398	95400	3.10%	0.306%
51	12.842	939	941	942 rBV	114611	152980	4.97%	0.490%
52	12.865	942	943	946 rVB2	898292	888272	28.84%	2.847%
53	12.945	947	950	951 rBV2	111217	183828	5.97%	0.589%
54	13.048	955	959	961 rVB2	178971	284905	9.25%	0.913%
55	13.116	963	965	966 rBV	94374	82653	2.68%	0.265%
56	13.151	966	968	969 rBV	174908	180978	5.88%	0.580%
57	13.242	974	976	977 rBV	74685	58519	1.90%	0.188%
58	13.277	977	979	981 rBV2	65438	66022	2.14%	0.212%
59	13.357	984	986	988 rBV2	127818	149661	4.86%	0.480%
60	13.551	1001	1003	1006 rBV	205231	230429	7.48%	0.739%
61	13.665	1010	1013	1014 rBV	188466	222259	7.22%	0.712%
62	13.699	1014	1016	1017 rVV	82441	159418	5.18%	0.511%
63	13.757	1020	1021	1025 rVB	166083	235395	7.64%	0.754%
64	13.917	1032	1035	1041 rVB2	1725246	3079859	100.00%	9.871%
65	14.019	1042	1044	1046 rBV	102678	94603	3.07%	0.303%
66	14.054	1046	1047	1050 rBV3	47790	94230	3.06%	0.302%
67	14.145	1053	1055	1056 rVB2	70580	74199	2.41%	0.238%
68	14.305	1067	1069	1070 rVV	128292	123391	4.01%	0.395%
69	14.339	1070	1072	1074 rVB	88191	79721	2.59%	0.256%
70	14.602	1093	1095	1096 rBV	71920	81806	2.66%	0.262%
71	14.762	1107	1109	1114 rBV3	76545	173101	5.62%	0.555%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121816\
Data File : BF091767.D
Acq On : 19 Dec 2016 6:14
Operator : UM/SJ
Sample : H6006-22DL 5X
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-2-0-5DL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	14.922	1121	1123	1128	rBV	746624	1514949	49.19%	4.856%
73	15.025	1130	1132	1134	rVB	154367	167140	5.43%	0.536%
74	15.208	1145	1148	1151	rVB	418466	566855	18.41%	1.817%
75	15.265	1151	1153	1155	rVV	576723	713430	23.16%	2.287%
76	15.322	1155	1158	1164	rVB2	1000714	1508077	48.97%	4.834%
77	16.363	1247	1249	1255	rVB4	81133	184513	5.99%	0.591%
78	16.671	1272	1276	1280	rVB2	267872	554076	17.99%	1.776%
79	16.820	1287	1289	1292	rBV	53488	121387	3.94%	0.389%
80	17.071	1307	1311	1317	rVB	200195	421177	13.68%	1.350%


Sum of corrected areas: 31200499

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121816\
Data File : BF091767.D
Acq On : 19 Dec 2016 6:14
Operator : UM/SJ
Sample : H6006-22DL 5X
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-2-0-5DL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

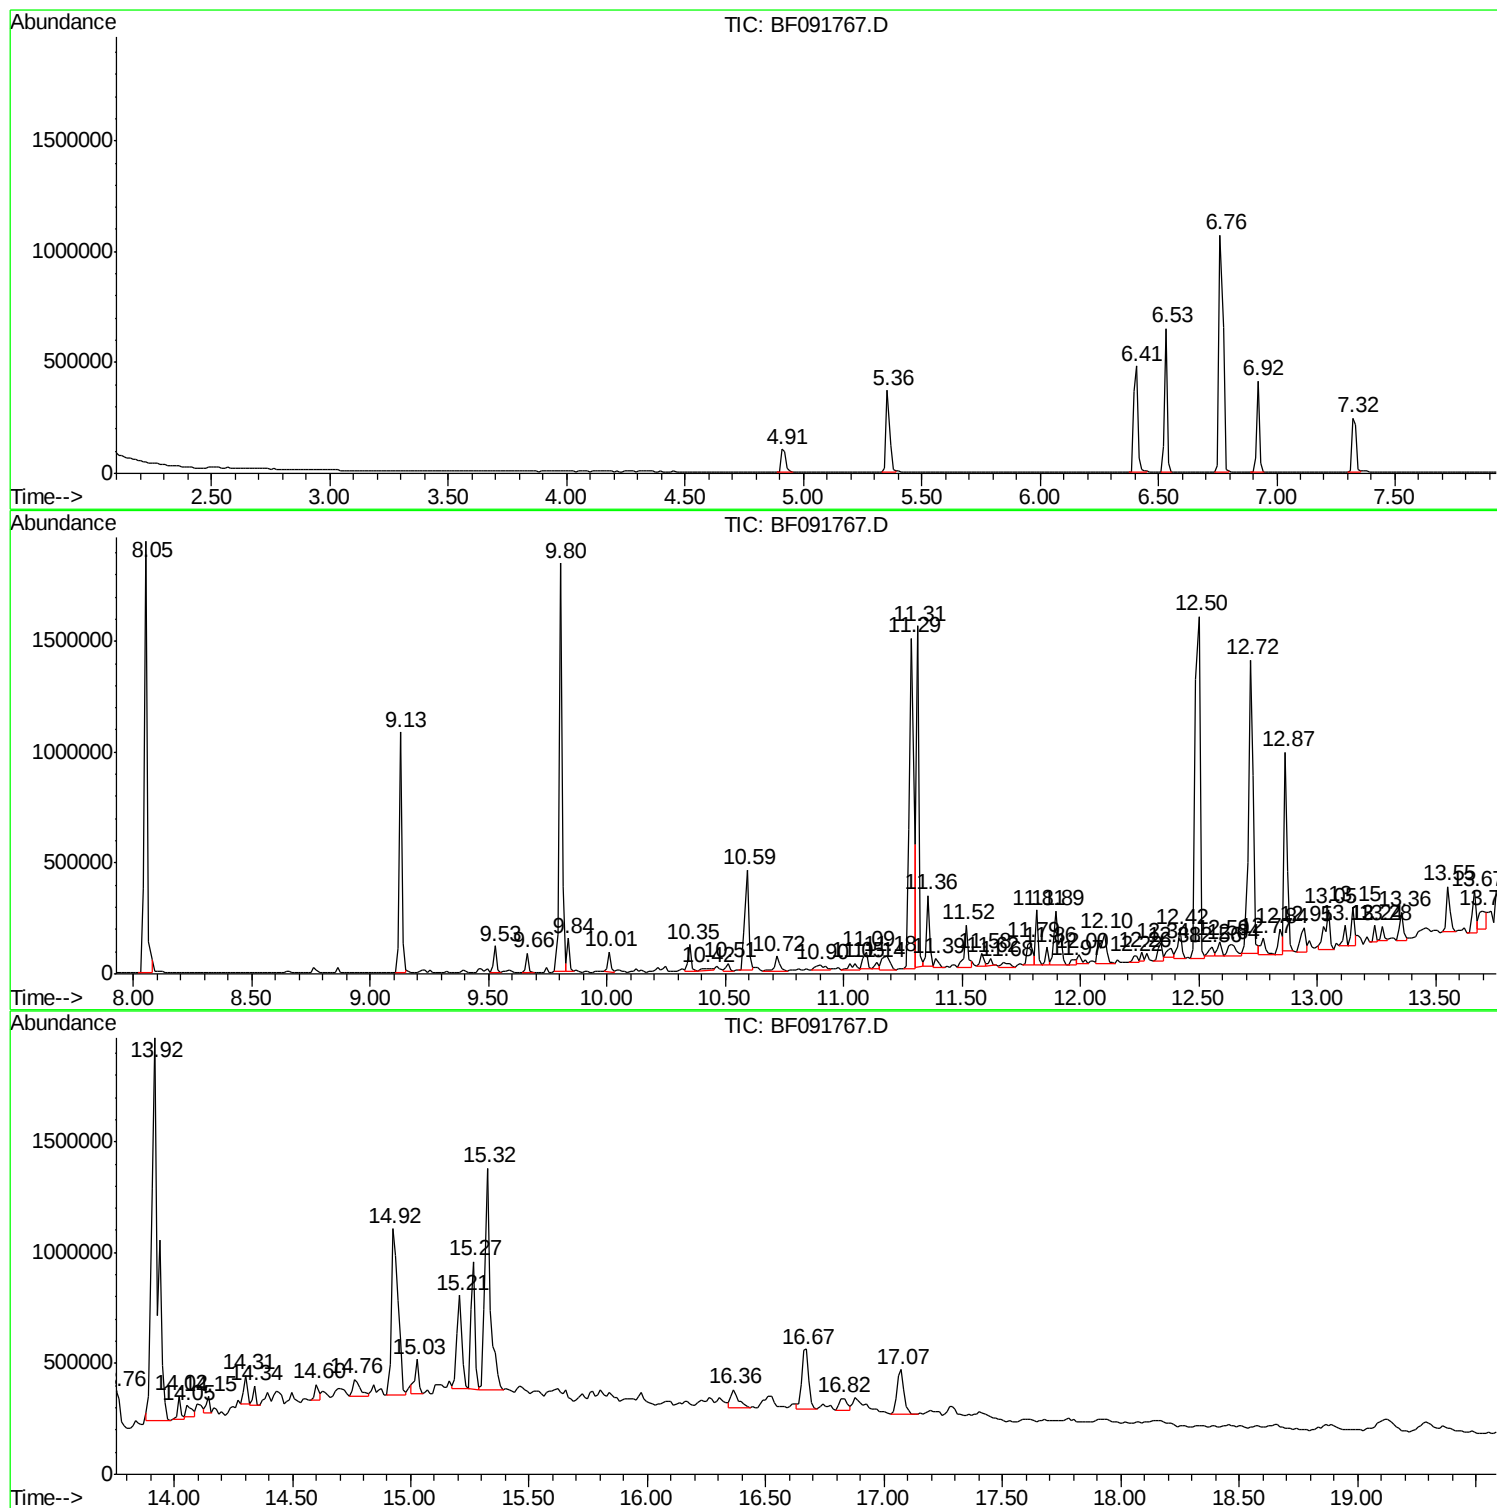

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF121816\
Data_File : BF091767.D
Acq_On : 19-Dec-2016 6:144
Operator : UM/SJJ
Sample : H6006-22DL_5XX
Misc :
ALS_Vial : 54 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
WC-2-0-5DL

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
