


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121816\
 Data File : BF091732.D
 Acq On : 18 Dec 2016 12:55
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 17 22:53:54 2016

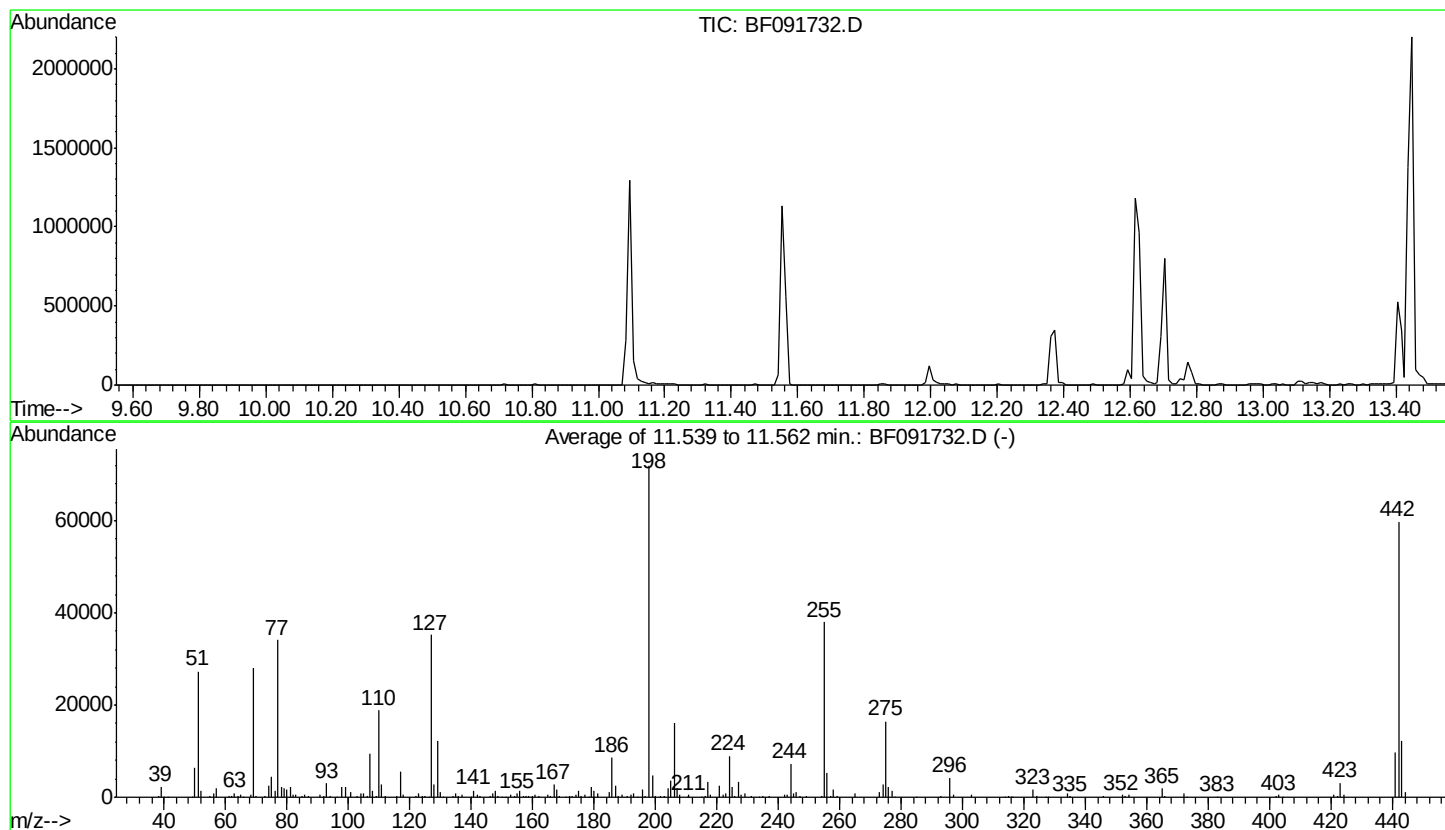

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	27351	PASS
68	69	0.00	2	1.7	463	PASS
69	198	0.00	100	38.9	28000	PASS
70	69	0.00	2	0.6	163	PASS
127	198	10	80	48.9	35184	PASS
197	198	0.00	2	0.3	232	PASS
198	198	100	100	100.0	71966	PASS
199	198	5	9	6.5	4643	PASS
275	198	10	60	22.9	16453	PASS
365	198	1	100	2.6	1882	PASS
441	442	0.01	24	16.1	9645	PASS
442	198	50	100	83.1	59812	PASS
443	442	15	24	20.3	12140	PASS