
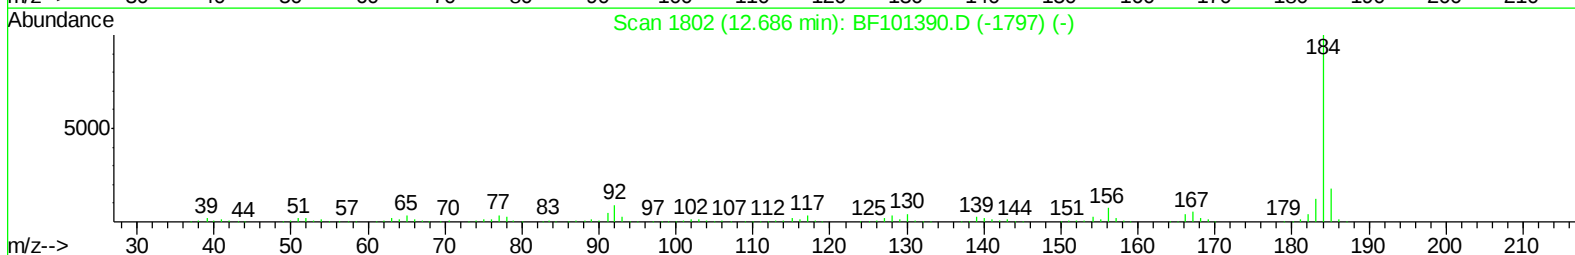
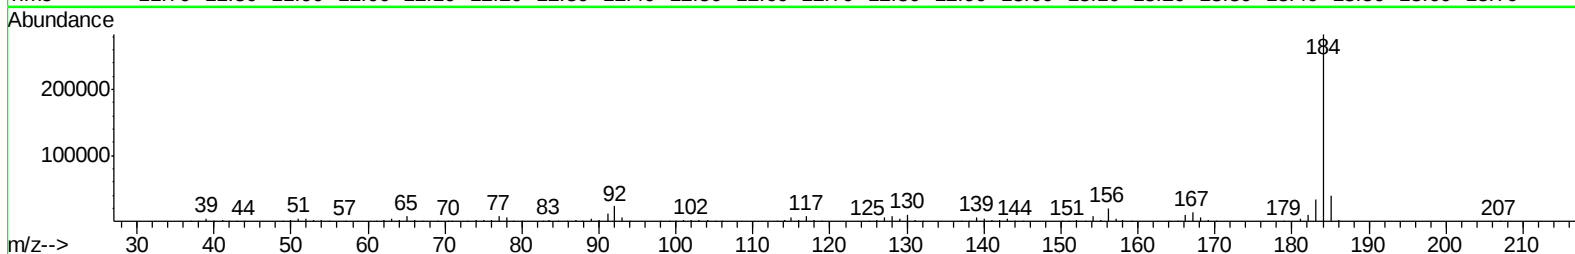


Data Path : Z:\HPCHEM1\BNA F\DATA\BF121817\
Data File : BF101498.D
Acq On : 19 Dec 2017 00:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 08:19:54 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 18 15:38:59 2017
Response via : Initial Calibration

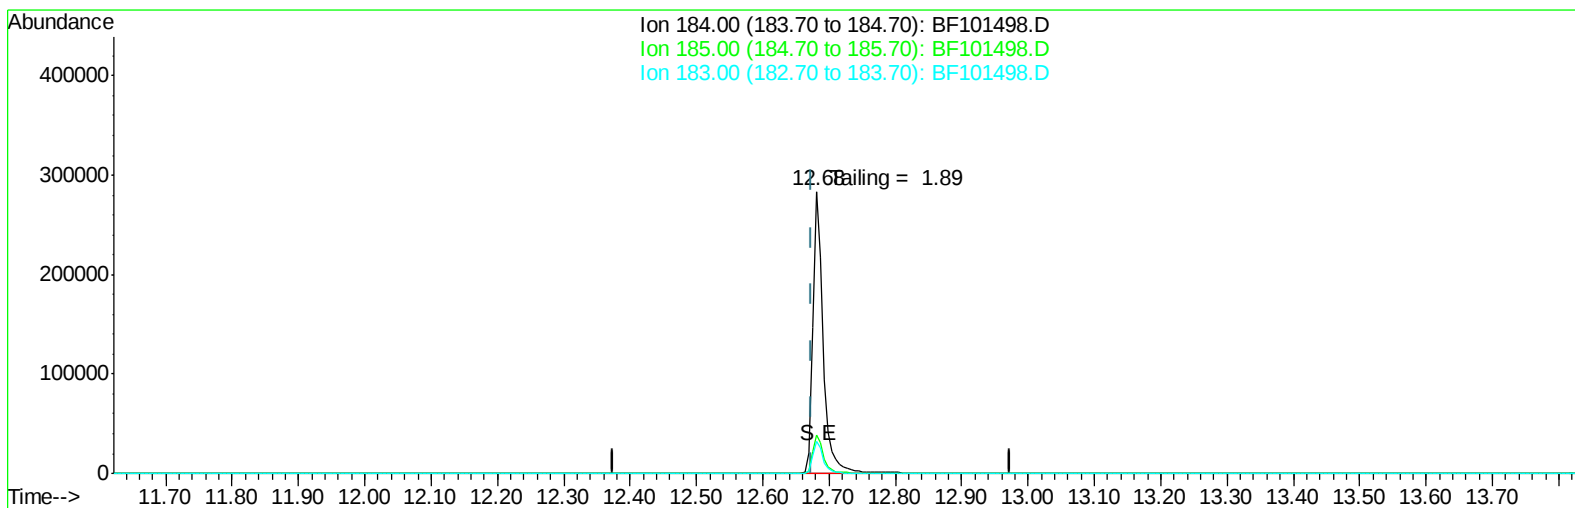

TIC: BF101498.D

(76) Benzidine




12.680min (+0.006) 0.00ng

response 311043

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.86
183.00	11.60	11.59
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121817\
Data File : BF101498.D
Acq On : 19 Dec 2017 00:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 08:19:54 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 18 15:38:59 2017
Response via : Initial Calibration

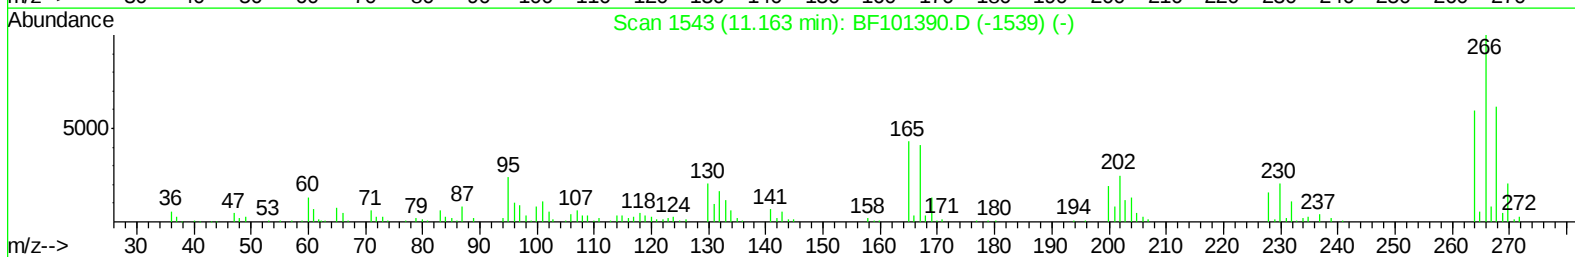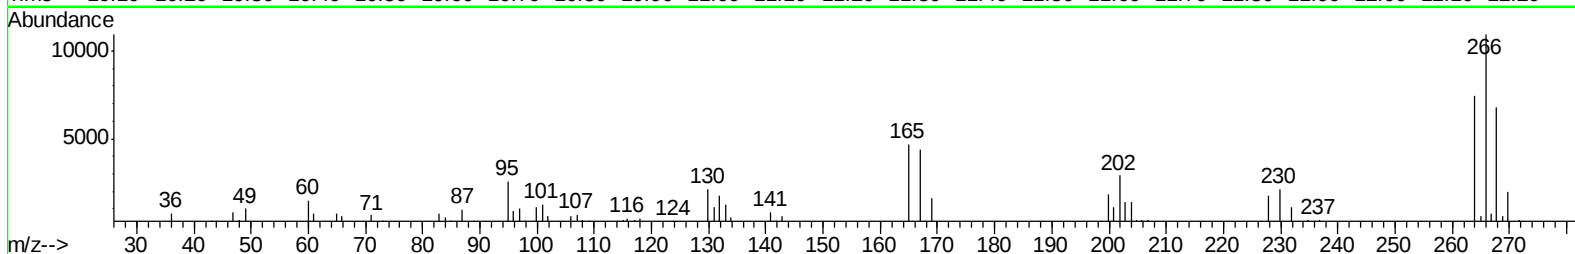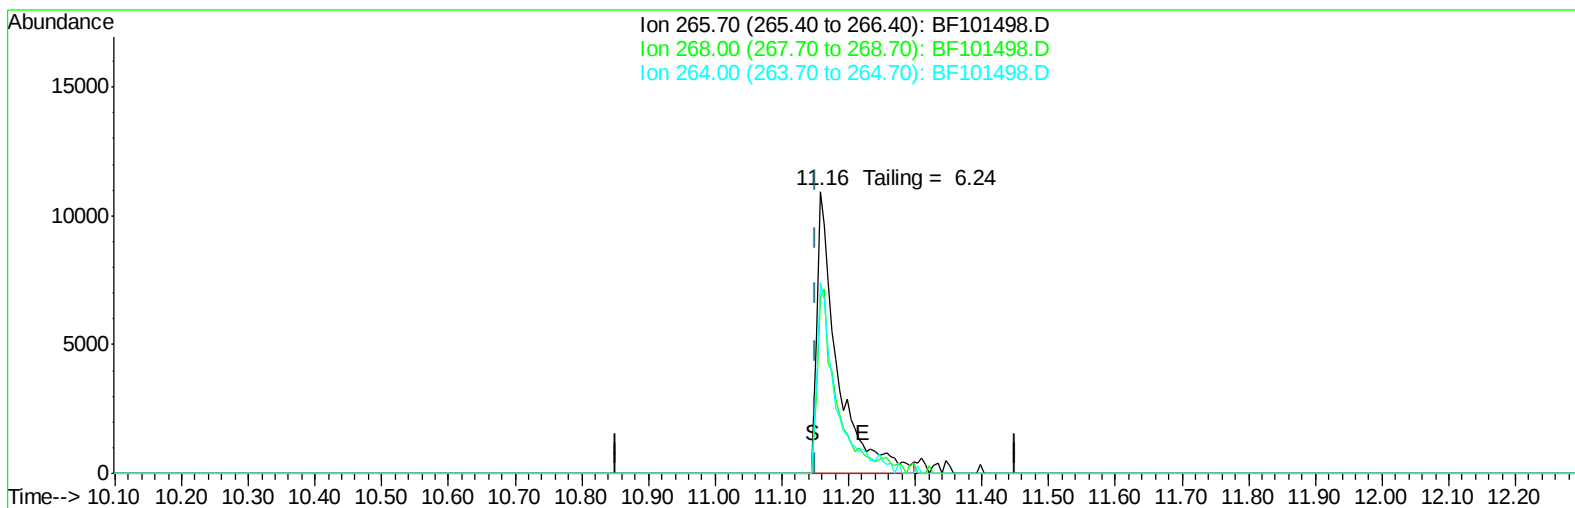

TIC: BF101498.D

(69) Pentachlorophenol (C)

11.157min (+0.006) 20475.45ng

response 23303

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.11
264.00	61.90	67.82
0.00	0.00	0.00