


Data Path : Z:\HPCHEM1\BNA_F\Data\BF121817\
 Data File : BF101472.D
 Acq On : 18 Dec 2017 10:53
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 18 15:38:59 2017

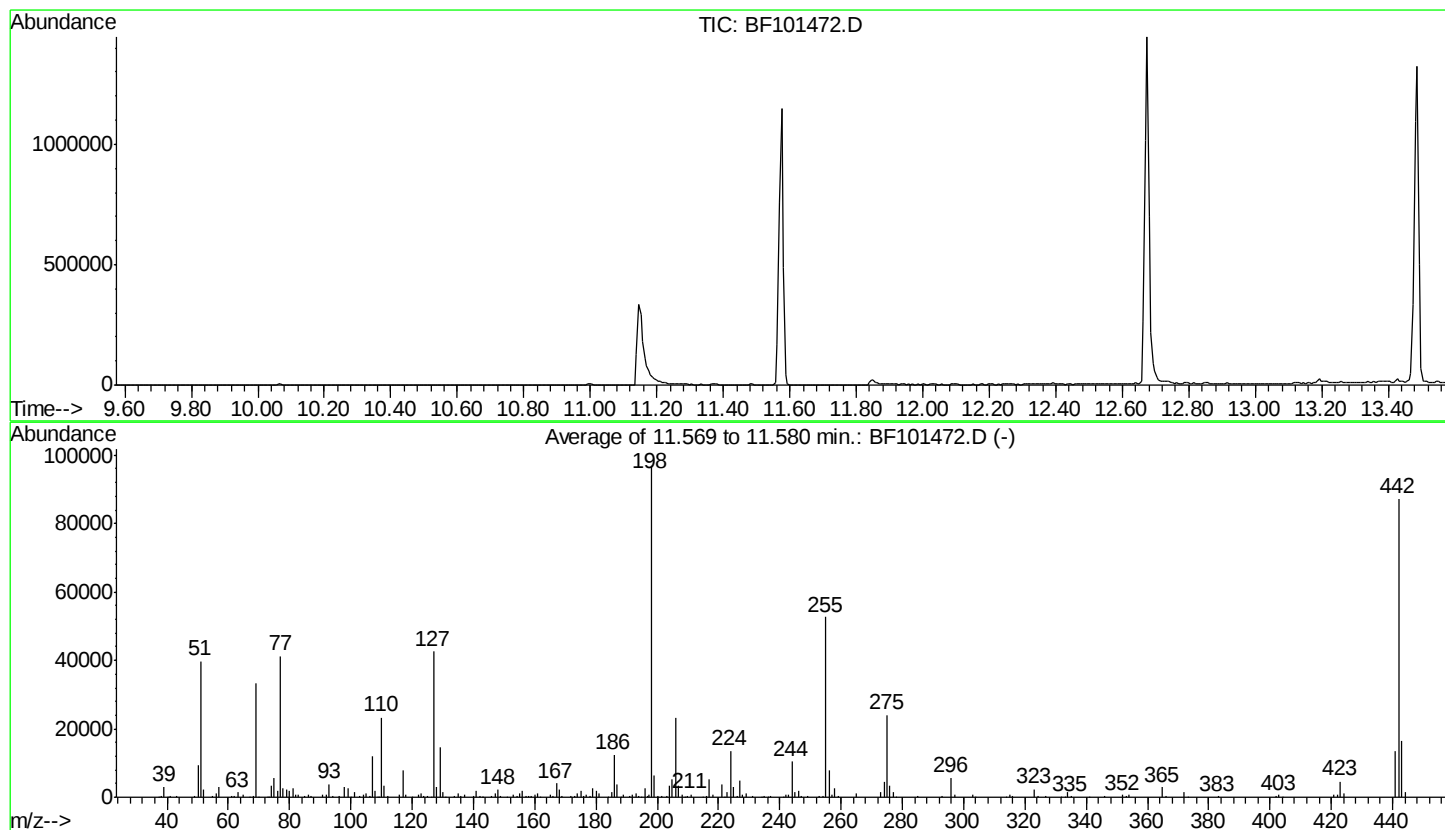

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	39853	PASS
68	69	0.00	2	1.7	551	PASS
69	198	0.00	100	34.3	33247	PASS
70	69	0.00	2	0.3	110	PASS
127	198	10	80	44.0	42632	PASS
197	198	0.00	2	0.7	670	PASS
198	198	100	100	100.0	96928	PASS
199	198	5	9	6.6	6379	PASS
275	198	10	60	24.8	24061	PASS
365	198	1	100	3.1	2985	PASS
441	443	0.01	100	81.3	13543	PASS
442	198	50	100	90.0	87202	PASS
443	442	15	24	19.1	16662	PASS