


Data Path : Z:\HPCHEM1\BNA_F\Data\BF121817\
 Data File : BF101498.D
 Acq On : 19 Dec 2017 00:06
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 18 15:38:59 2017

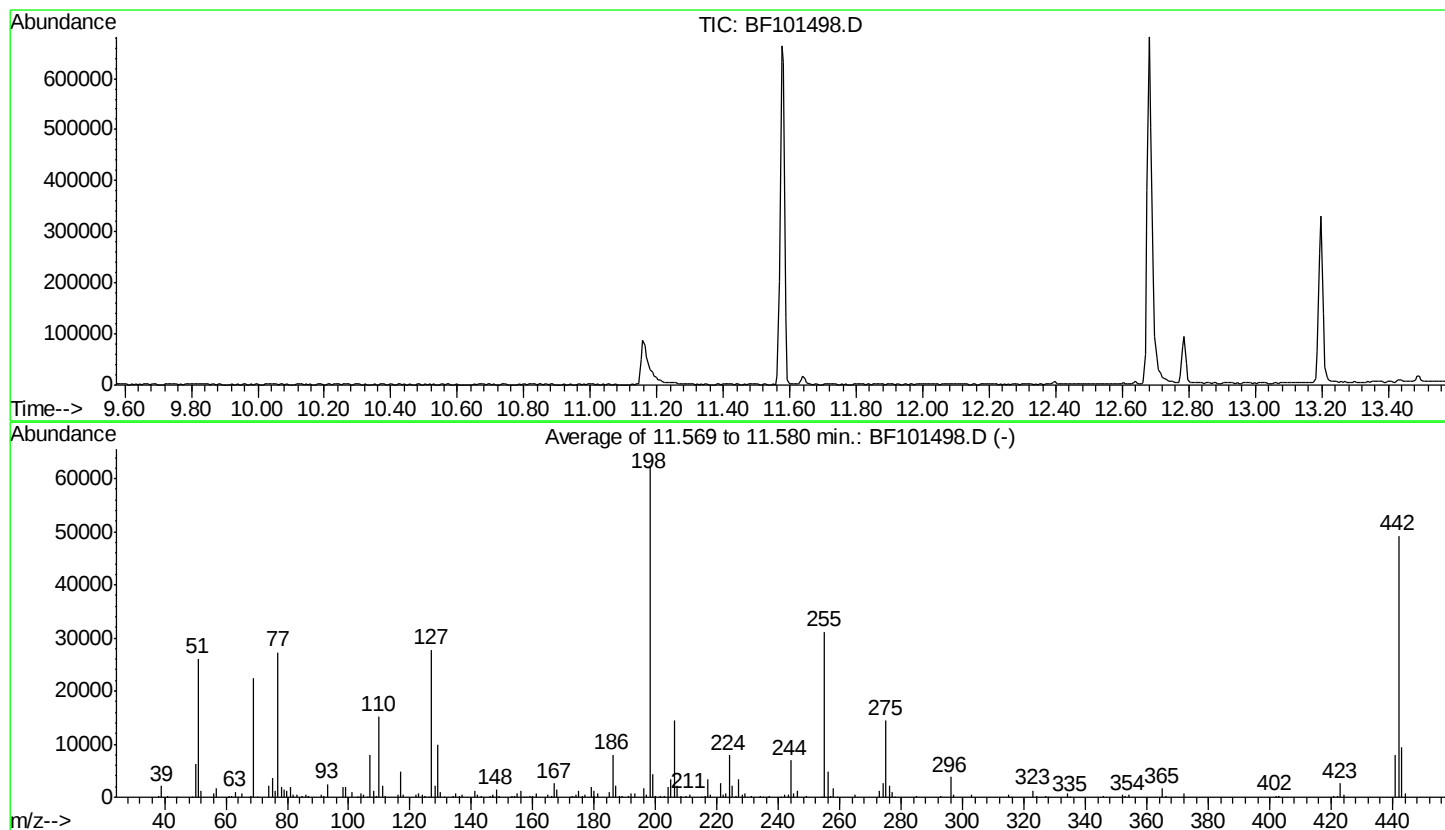

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	26042	PASS
68	69	0.00	2	1.3	282	PASS
69	198	0.00	100	36.1	22526	PASS
70	69	0.00	2	0.5	102	PASS
127	198	10	80	44.5	27808	PASS
197	198	0.00	2	0.8	517	PASS
198	198	100	100	100.0	62450	PASS
199	198	5	9	6.9	4316	PASS
275	198	10	60	23.1	14442	PASS
365	198	1	100	2.6	1652	PASS
441	443	0.01	100	84.0	7901	PASS
442	198	50	100	78.9	49282	PASS
443	442	15	24	19.1	9407	PASS