
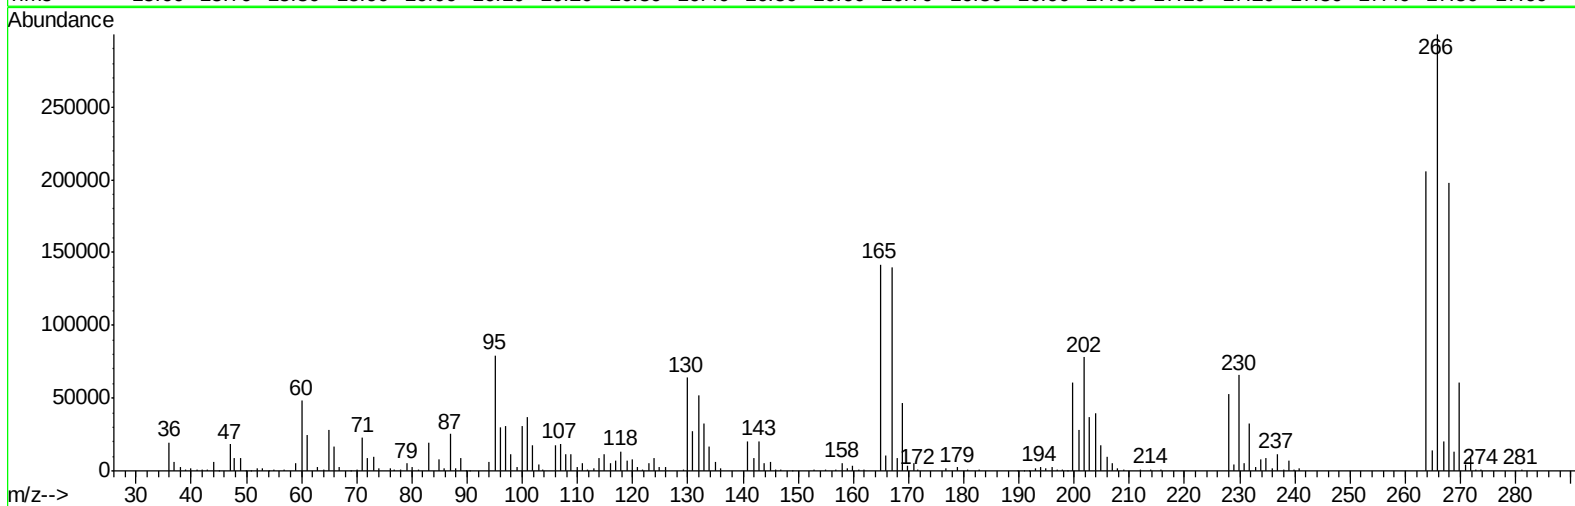


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN121819\
 Data File : BN009019.D
 Acq On : 18 Dec 2019 14:25
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 05:52:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN120919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 19 00:50:46 2019
 Response via : Initial Calibration

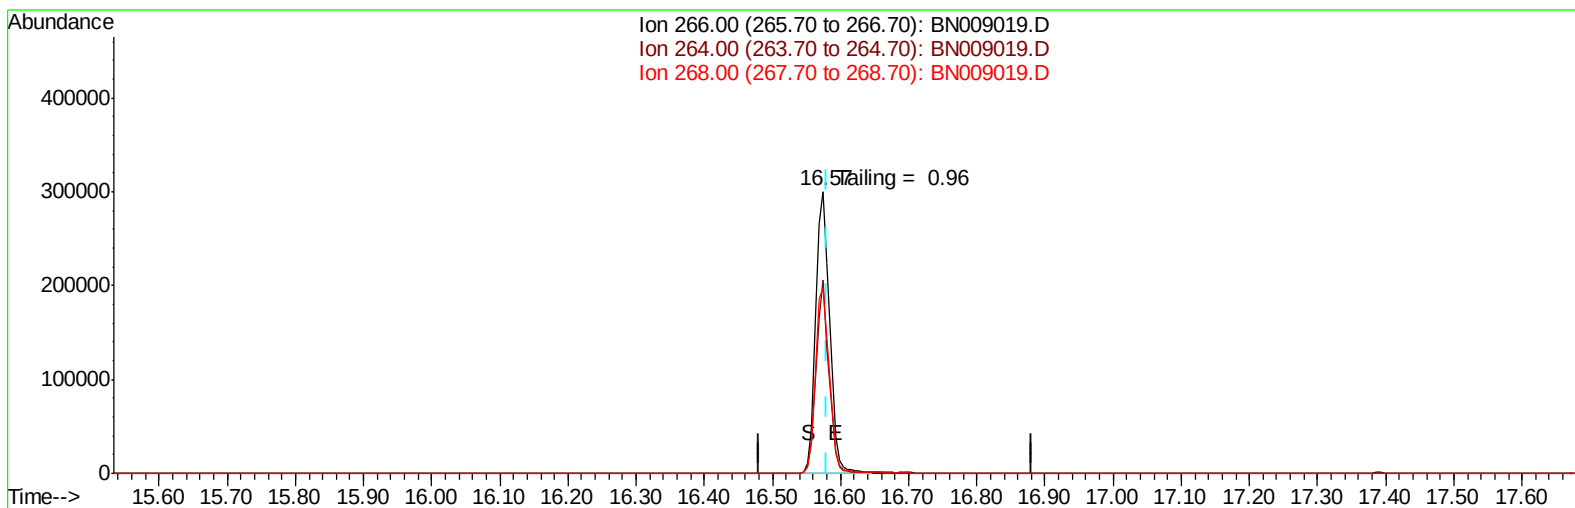

TIC: BN009019.D

(22) Pentachlorophenol

16.575min (-0.007) 0.00ng

response 427935

Ion	Exp%	Act%
266.00	100	100
264.00	64.40	68.52
268.00	66.40	66.09
0.00	0.00	0.00