
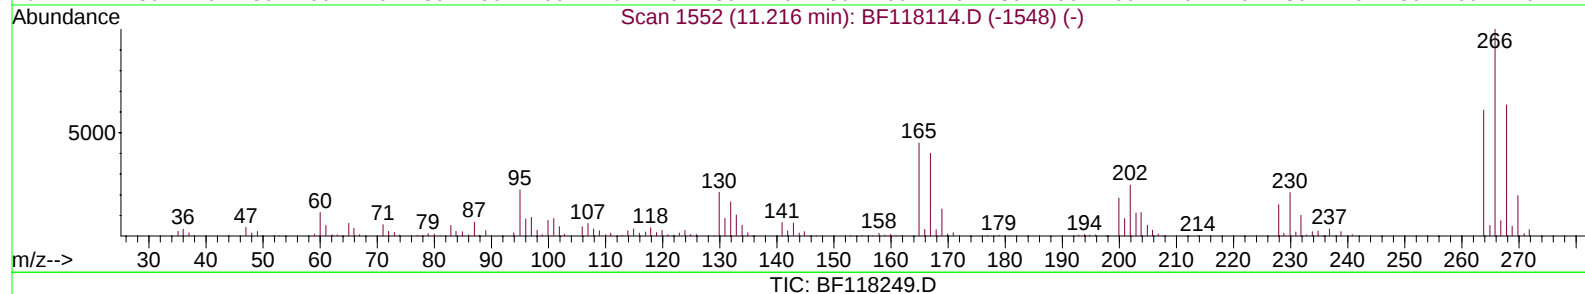
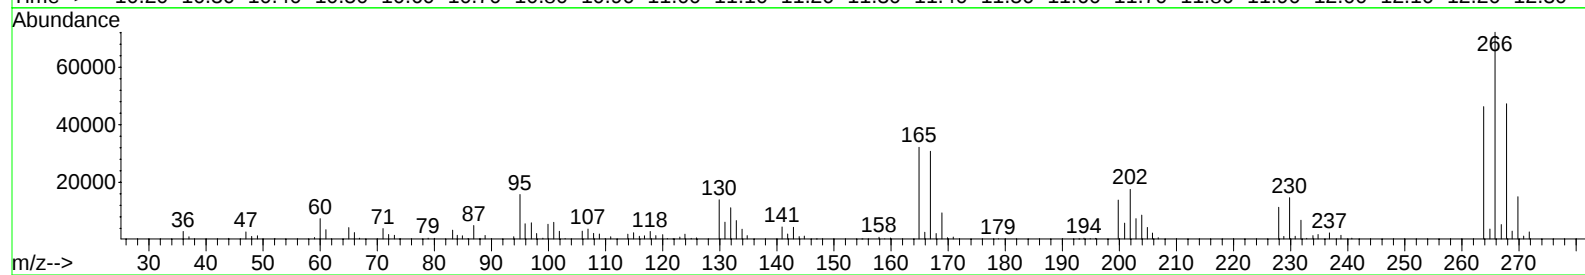


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF121819\
Data File : BF118249.D
Acq On : 18 Dec 2019 10:13
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 18 17:41:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 17:34:43 2019
Response via : Initial Calibration

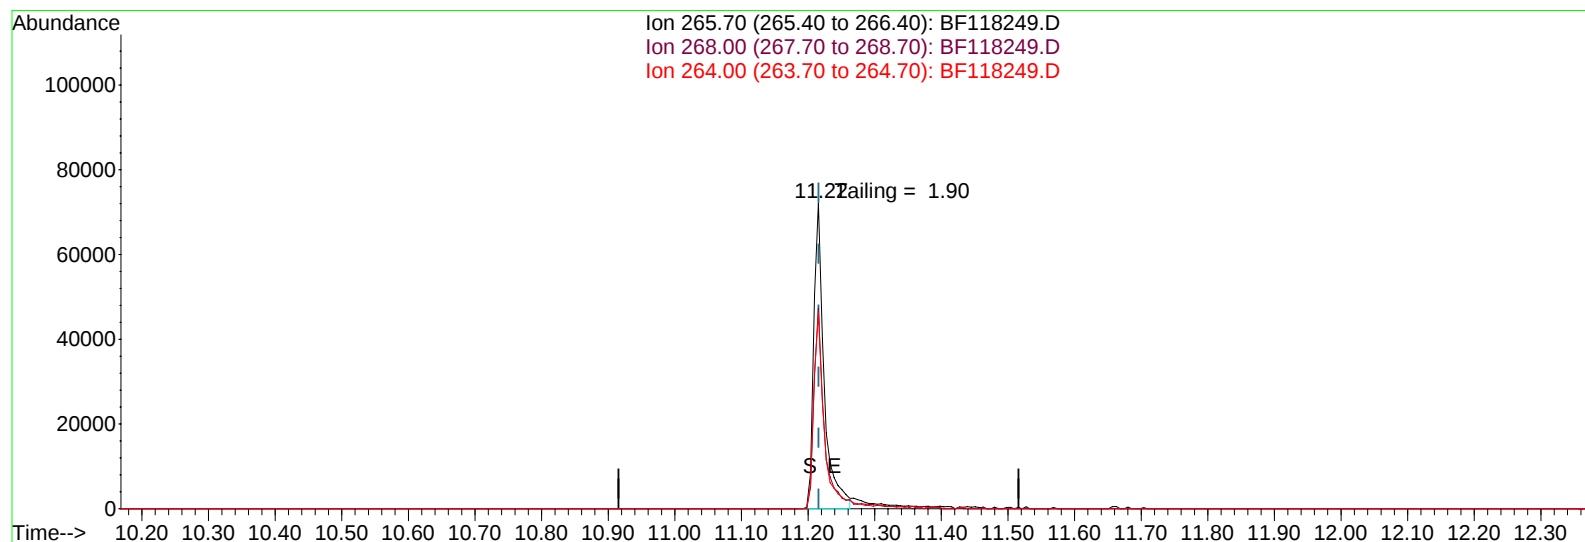

(70) Pentachlorophenol (C)




11.216min (-0.000) 31224.99ng

response 85824

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	65.57
264.00	60.90	64.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF121819\
 Data File : BF118249.D
 Acq On : 18 Dec 2019 10:13
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 18 17:41:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 17:34:43 2019
 Response via : Initial Calibration

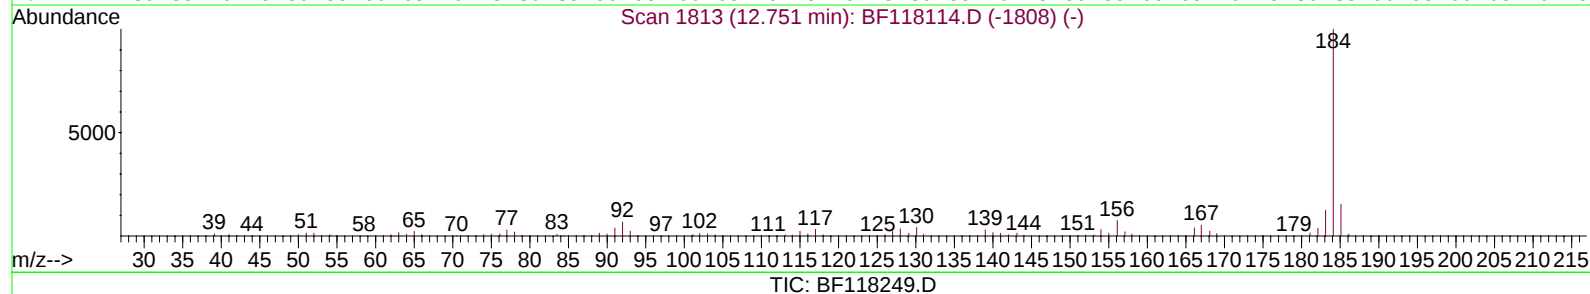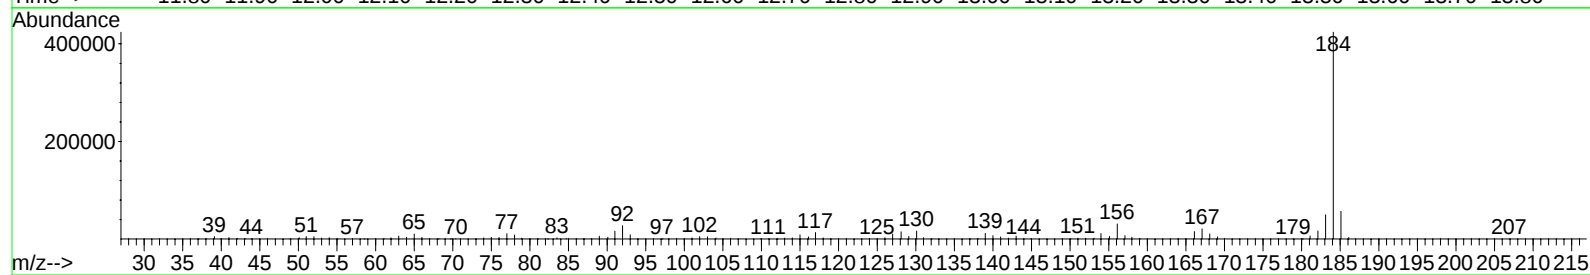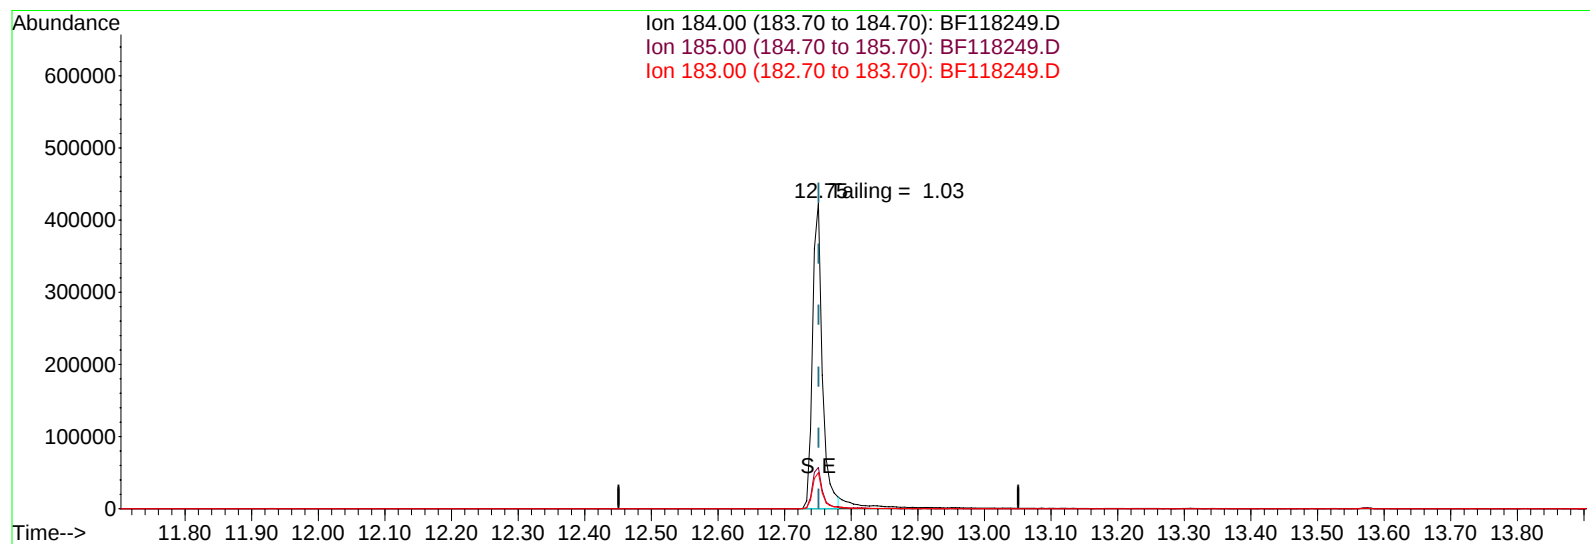

(77) Benzidine

12.751min (-0.000) 0.00ng

response 466209

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	13.49
183.00	12.40	11.77
0.00	0.00	0.00