

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121819\
 Data File : BF118271.D
 Acq On : 18 Dec 2019 20:58
 Operator : JU
 Sample : K6357-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PF-03

Quant Time: Dec 19 03:59:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 17:34:43 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	94575	20.00	ng	-0.01
21) Naphthalene-d8	8.15	136	368836	20.00	ng	-0.01
39) Acenaphthene-d10	9.91	164	190478	20.00	ng	-0.01
64) Phenanthrene-d10	11.40	188	362066	20.00	ng	0.00
76) Chrysene-d12	14.06	240	227959	20.00	ng	-0.01
87) Perylene-d12	15.54	264	218291	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	780201	144.49	ng	0.00
7) Phenol-d6	6.49	99	990076	151.59	ng	0.00
23) Nitrobenzene-d5	7.42	82	586918	89.52	ng	-0.02
42) 2,4,6-Tribromophenol	10.70	330	323140	139.65	ng	-0.01
45) 2-Fluorobiphenyl	9.23	172	1169487	93.43	ng	-0.01
79) Terphenyl-d14	12.99	244	1296470	97.80	ng	-0.01
Target Compounds						
10) Phenol	6.50	94	25293	3.396	ng	97
50) Dimethylphthalate	9.62	163	78033	5.546	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121819\
Data File : BF118271.D
Acq On : 18 Dec 2019 20:58
Operator : JU
Sample : K6357-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PF-03

Quant Time: Dec 19 03:59:25 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 17:34:43 2019
Response via : Initial Calibration

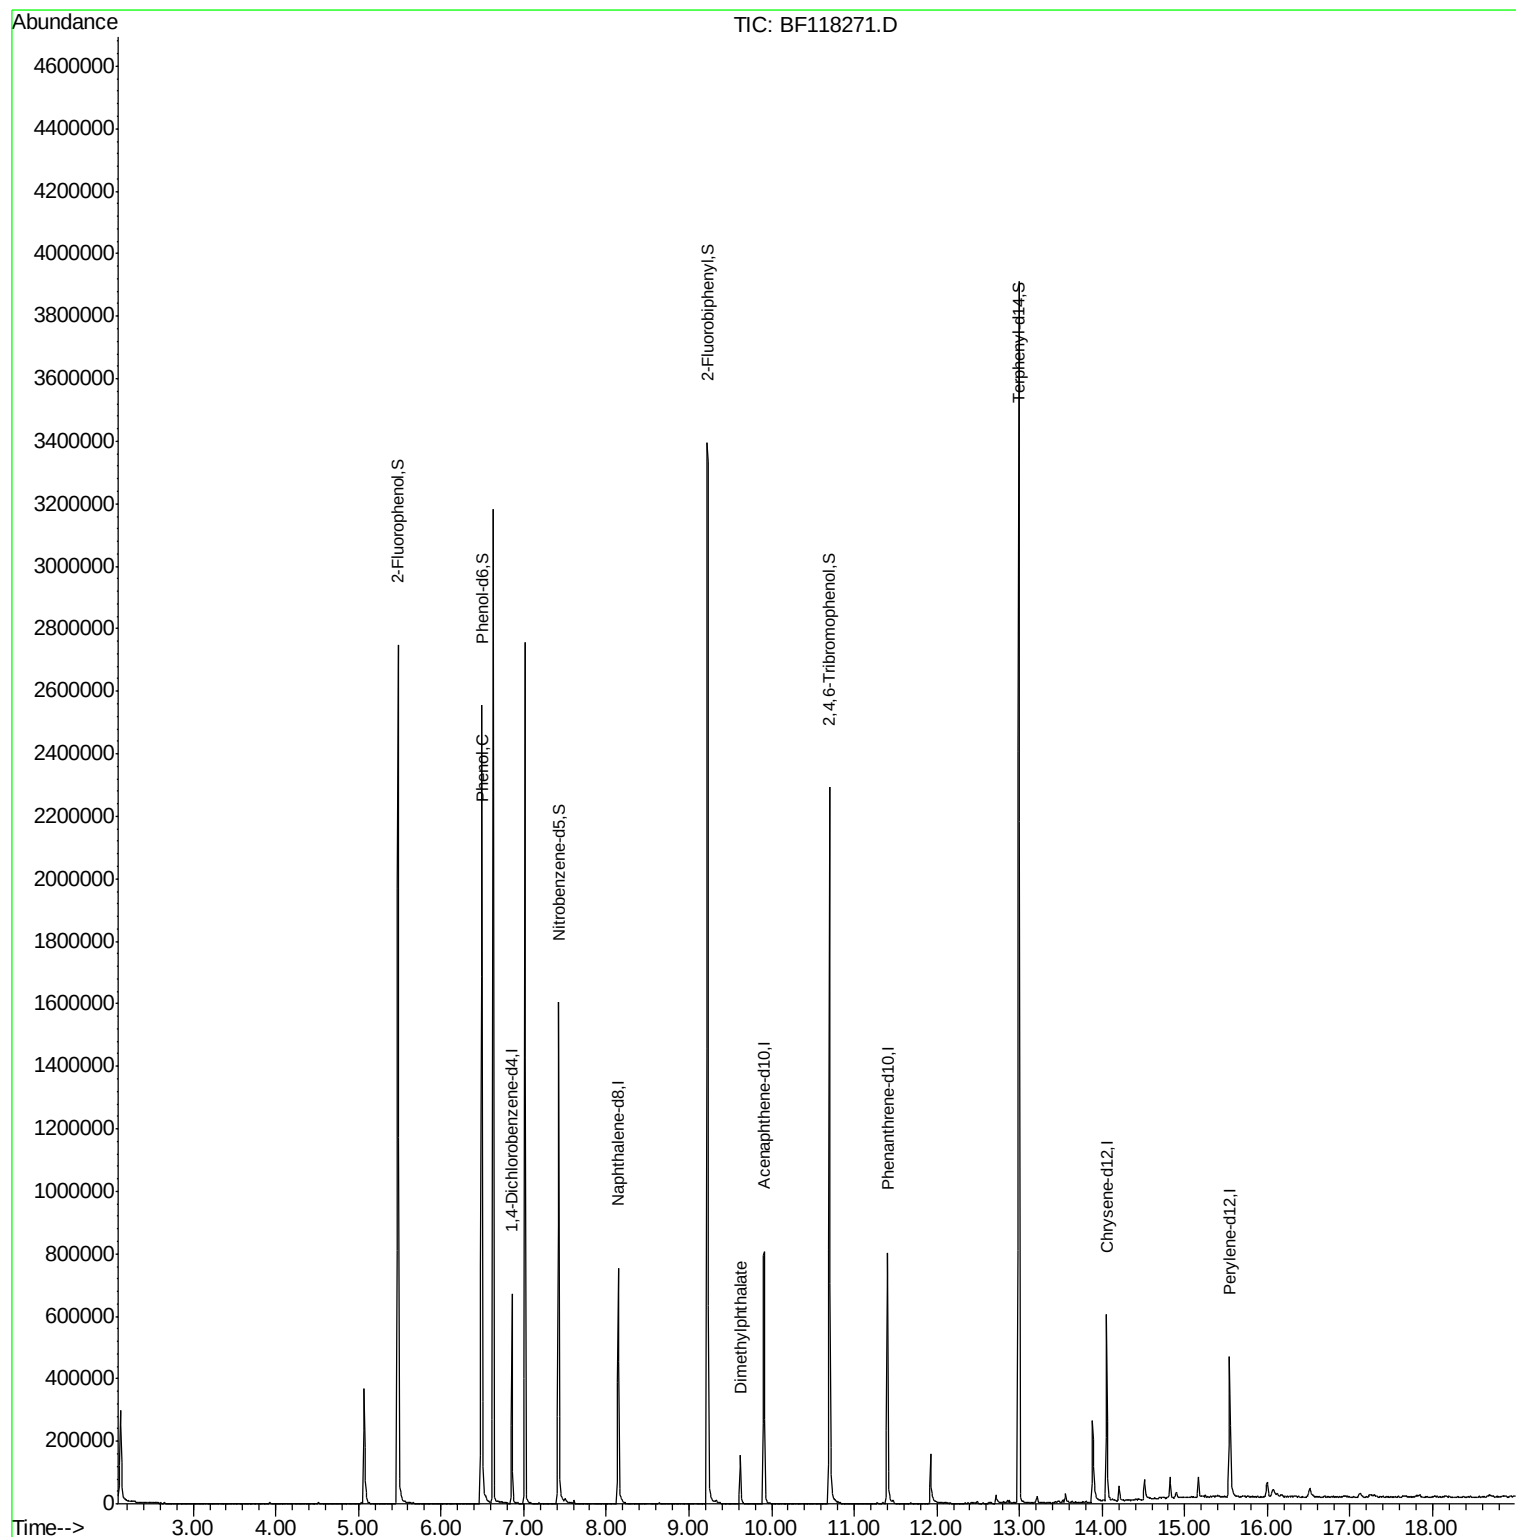

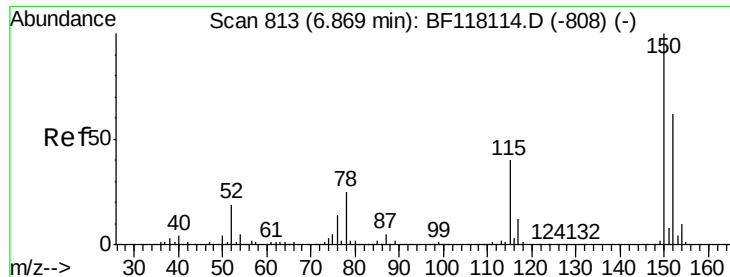


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.86 min Scan# 811
Delta R.T. -0.01 min
Lab File: BF118271.D
Acq: 18 Dec 2019 20:58

Instrument :
BNA_F
ClientSampled :
PF-03

Tot Ion:152 Resp: 94575
Ion Ratio Lower Upper
152 100
150 156.8 128.3 192.5
115 61.1 51.1 76.7

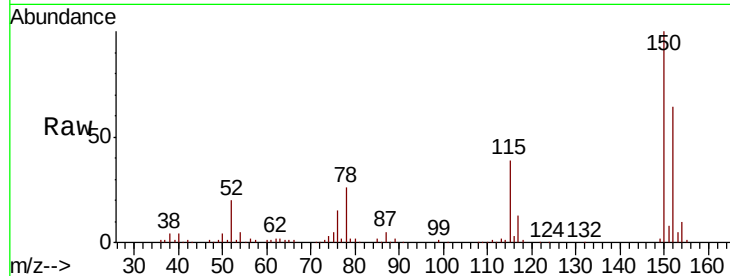


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

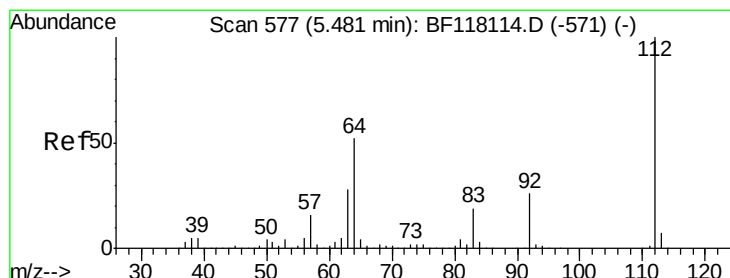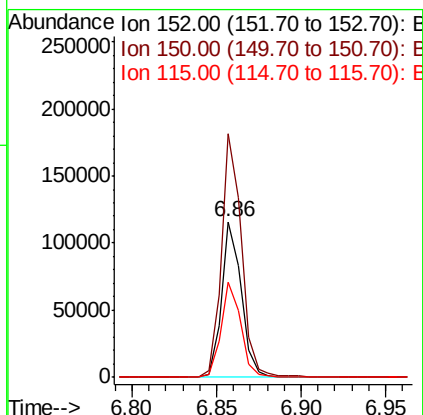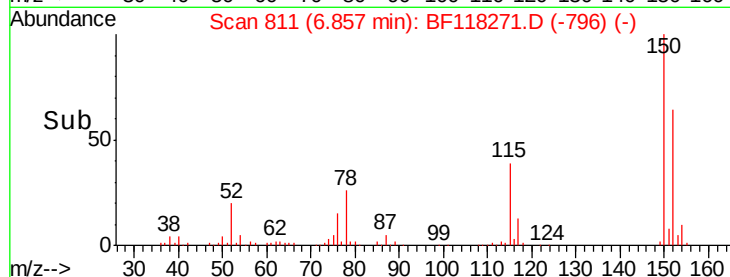



#5


2-Fluorophenol
Concen: 144.488 ng
RT: 5.48 min Scan# 577
Delta R.T. -0.00 min
Lab File: BF118271.D
Acq: 18 Dec 2019 20:58

Tgt Ion:112 Resp: 780201
Ion Ratio Lower Upper
112 100
64 52.3 41.3 61.9
63 29.0 22.4 33.6

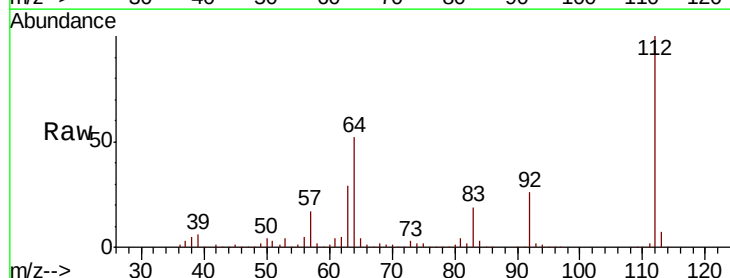

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

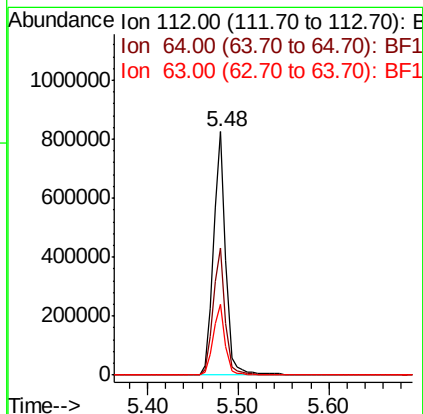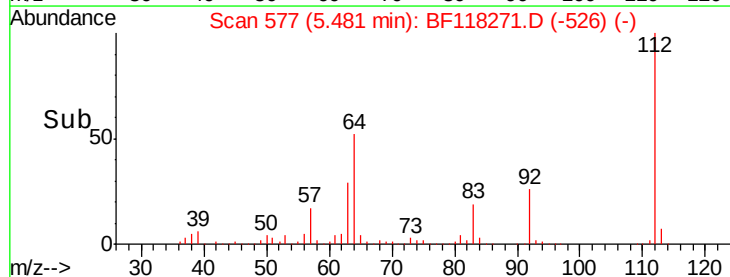

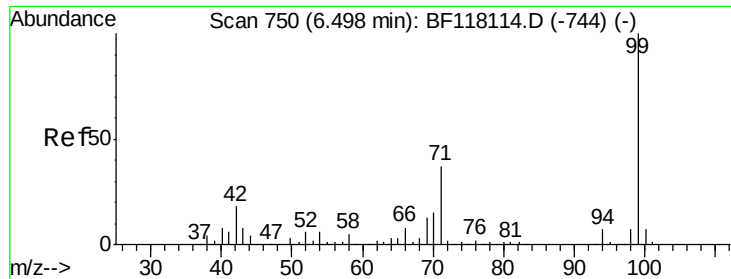

#7

Phenol-d6

Concen: 151.592 ng

RT: 6.49 min Scan# 749

Delta R.T. -0.01 min

Lab File: BF118271.D

Acq: 18 Dec 2019 20:58

Instrument :

BNA_F

ClientSampleId :

PF-03


Tot Ion: 99 Resp: 990076

Ion Ratio Lower Upper




99 100

42 18.0 14.1 21.1

71 37.6 29.7 44.5

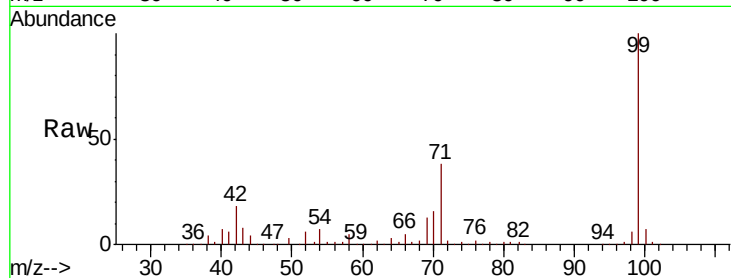

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

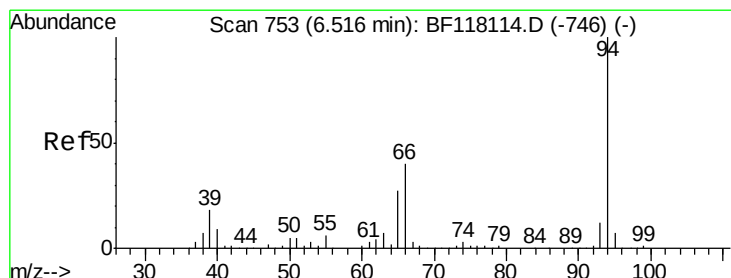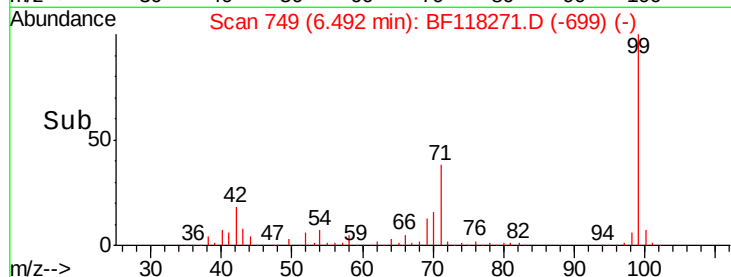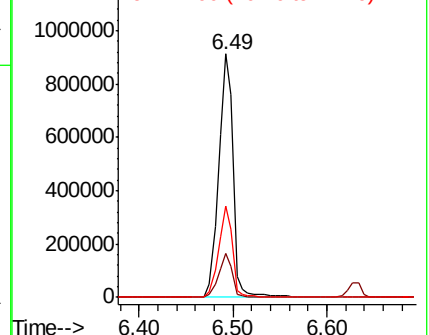

#10

Phenol

Concen: 3.396 ng

RT: 6.50 min Scan# 751

Delta R.T. -0.01 min

Lab File: BF118271.D

Acq: 18 Dec 2019 20:58


Tgt Ion: 94 Resp: 25293

Ion Ratio Lower Upper



94 100


65 28.6 7.3 47.3

66 42.7 20.2 60.2

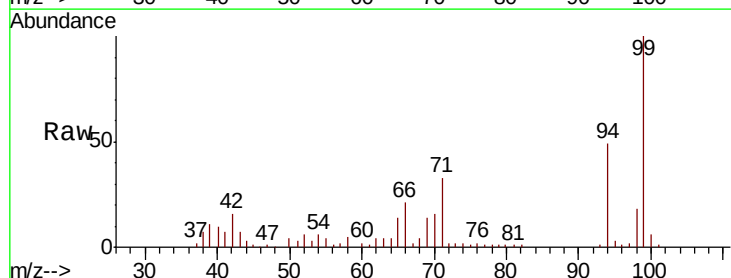

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

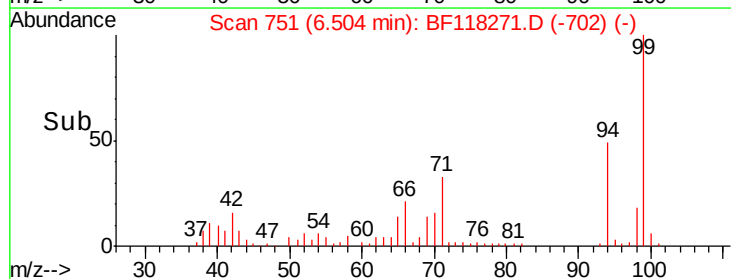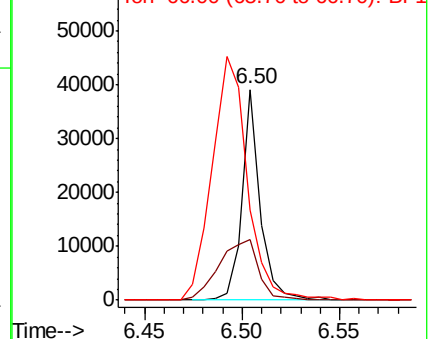

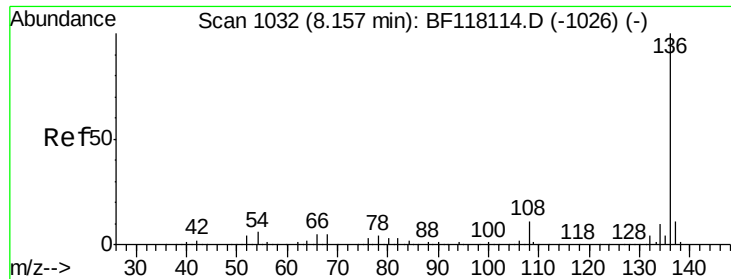

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.15 min Scan# 1030

Delta R.T. -0.01 min

Lab File: BF118271.D

Acq: 18 Dec 2019 20:58

Instrument :

BNA_F

ClientSampleId :

PF-03

Tot Ion:136 Resp: 368836



Ion Ratio Lower Upper

136 100

137 10.9 9.0 13.6

54 5.8 5.0 7.6

68 4.5 3.8 5.8

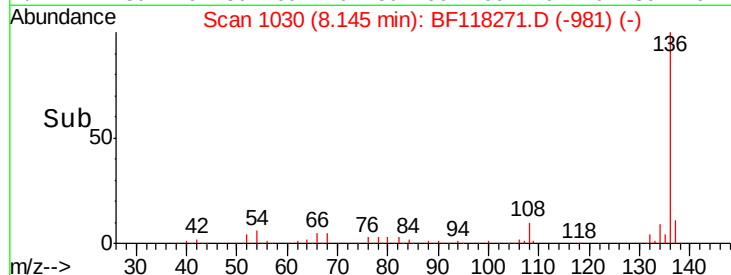
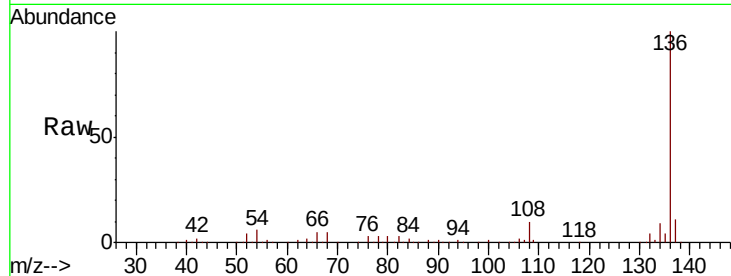


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

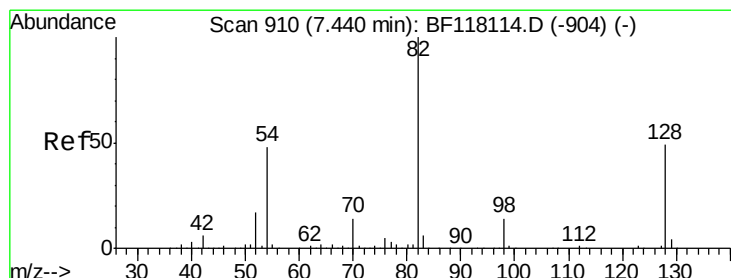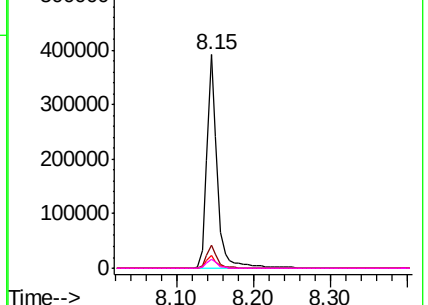

#23

Nitrobenzene-d5

Concen: 89.521 ng

RT: 7.42 min Scan# 907

Delta R.T. -0.02 min

Lab File: BF118271.D

Acq: 18 Dec 2019 20:58



Tgt Ion: 82 Resp: 586918

Ion Ratio Lower Upper

82 100

128 47.5 39.1 58.7


54 48.0 38.2 57.2

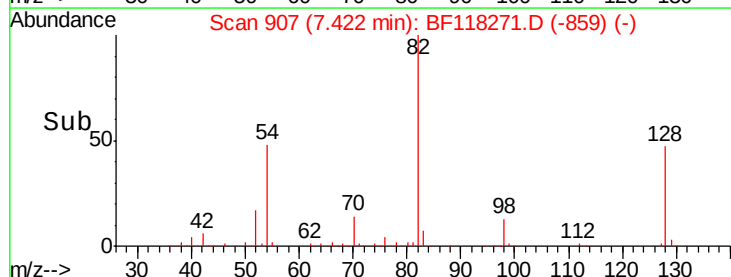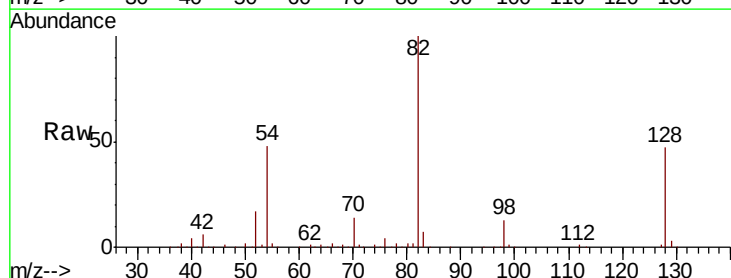


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

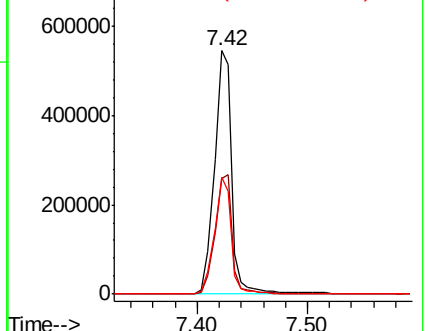

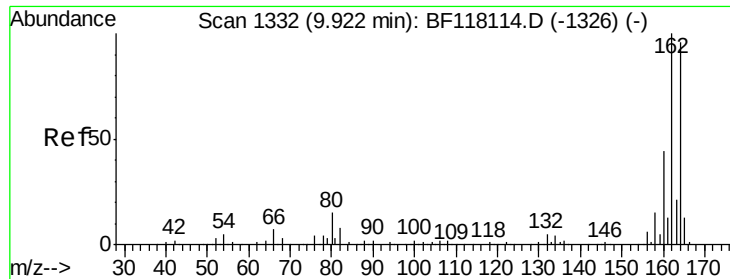

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.91 min Scan# 1330

Delta R.T. -0.01 min

Lab File: BF118271.D

Acq: 18 Dec 2019 20:58

Instrument :

BNA_F

ClientSampled :

PF-03



Tot Ion:164 Resp: 190478

Ion Ratio Lower Upper

164 100

162 100.6 83.4 125.0



160 45.2 36.6 54.8

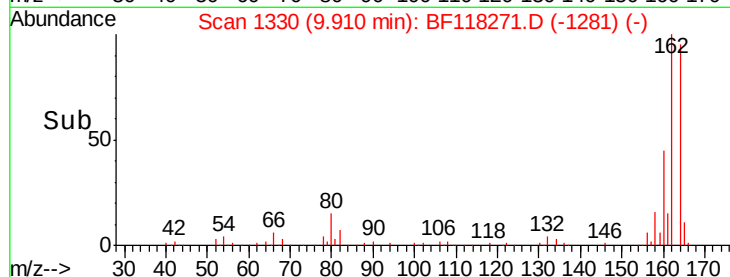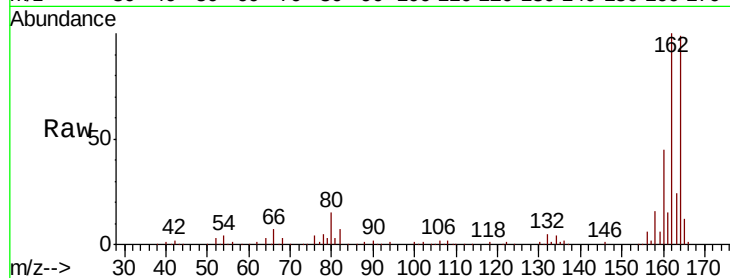

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

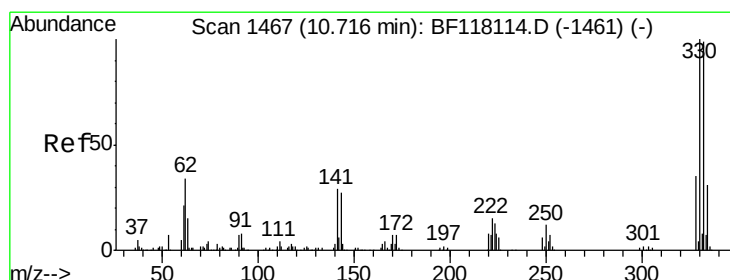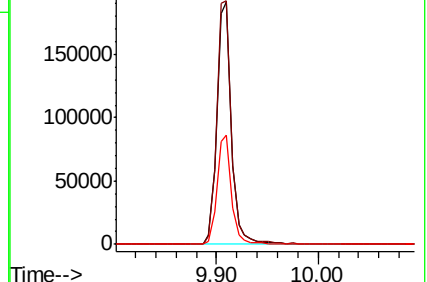

#42

2,4,6-Tribromophenol

Concen: 139.648 ng

RT: 10.70 min Scan# 1465

Delta R.T. -0.01 min

Lab File: BF118271.D

Acq: 18 Dec 2019 20:58



Tgt Ion:330 Resp: 323140

Ion Ratio Lower Upper

330 100

332 97.5 78.1 117.1


141 32.6 26.9 40.3

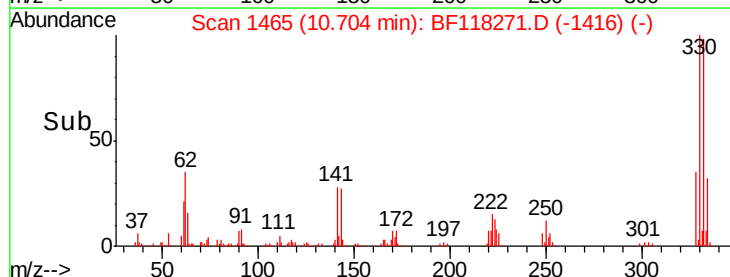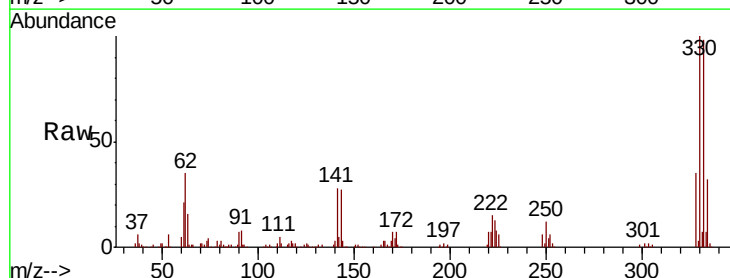


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

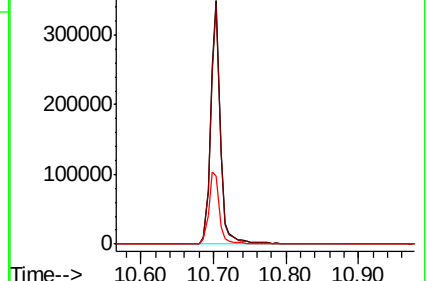


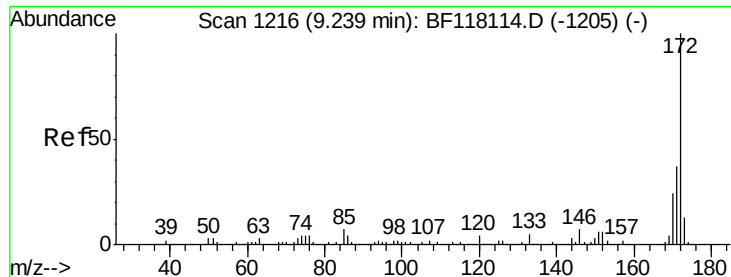




#45
2-Fluorobiphenyl
Concen: 93.425 ng
RT: 9.23 min Scan# 1214
Delta R.T. -0.01 min
Lab File: BF118271.D
Acq: 18 Dec 2019 20:58

Instrument :
BNA_F
ClientSampleId :
PF-03

Tot Ion:172 Resp: 1169487
Ion Ratio Lower Upper
172 100
171 35.4 29.2 43.8
170 23.6 19.4 29.2

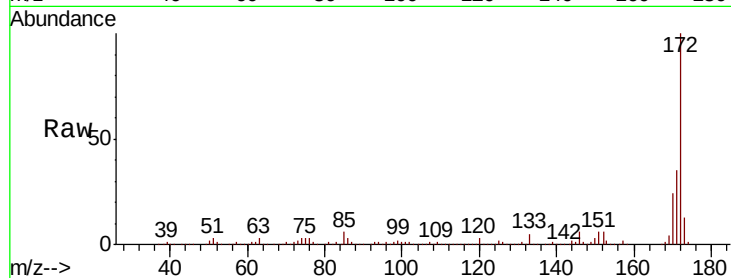


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

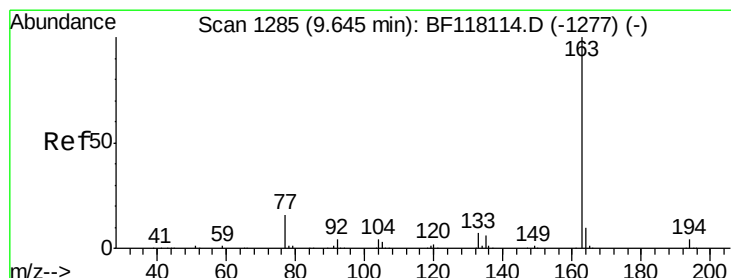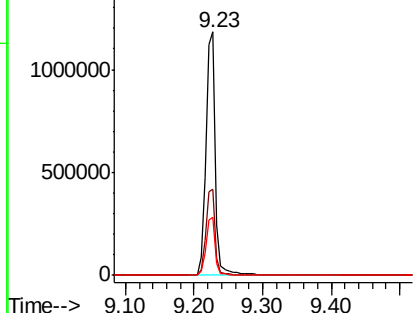
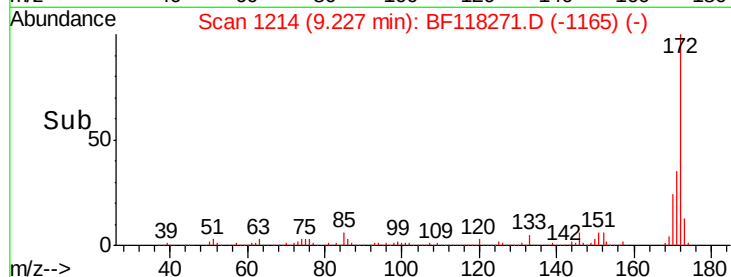



#50
Dimethylphthalate
Concen: 5.546 ng
RT: 9.62 min Scan# 1281
Delta R.T. -0.02 min
Lab File: BF118271.D
Acq: 18 Dec 2019 20:58

Tgt Ion:163 Resp: 78033
Ion Ratio Lower Upper
163 100
194 4.0 3.1 4.7
164 10.2 7.7 11.5

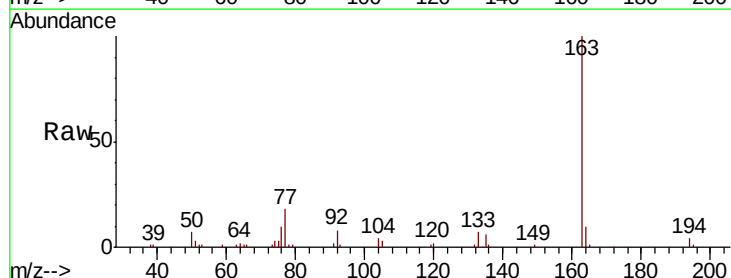

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E



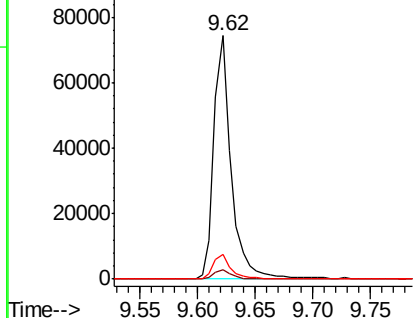
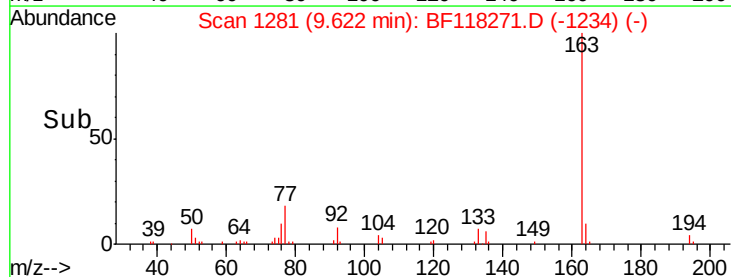


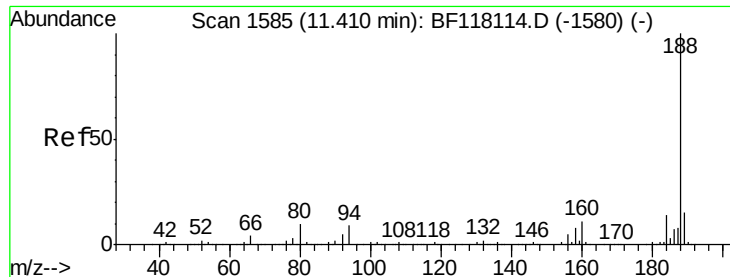

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.40 min Scan# 1584
Delta R.T. -0.01 min
Lab File: BF118271.D
Acq: 18 Dec 2019 20:58




Instrument :
BNA_F
ClientSampleId :
PF-03


Tot Ion:188 Resp: 362066
Ion Ratio Lower Upper
188 100
94 7.0 7.1 10.7#
80 7.6 7.9 11.9#

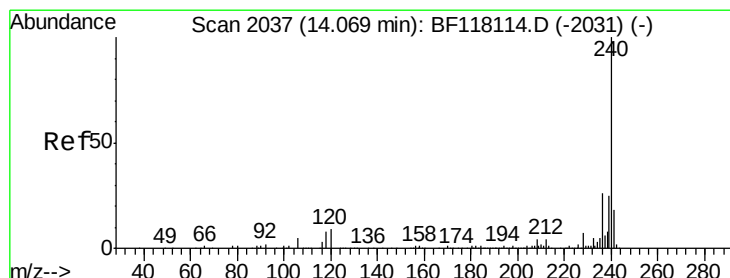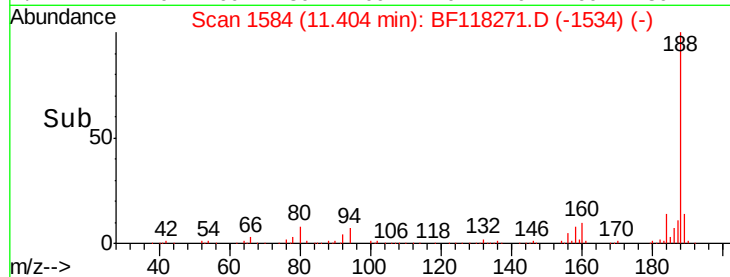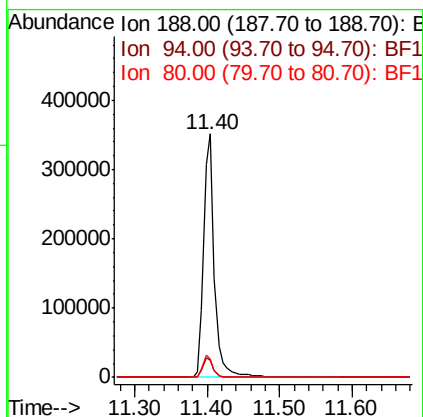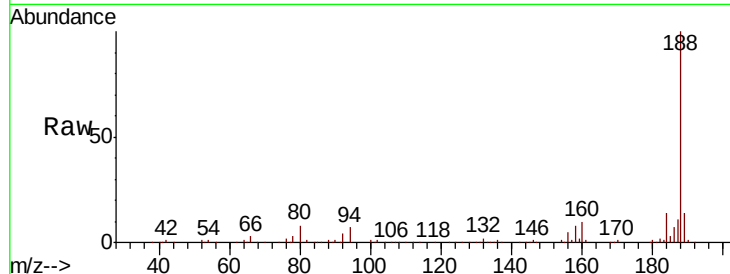

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.06 min Scan# 2035
Delta R.T. -0.01 min
Lab File: BF118271.D
Acq: 18 Dec 2019 20:58

Tgt Ion:240 Resp: 227959
Ion Ratio Lower Upper
240 100
120 9.4 7.1 10.7
236 26.2 21.0 31.6

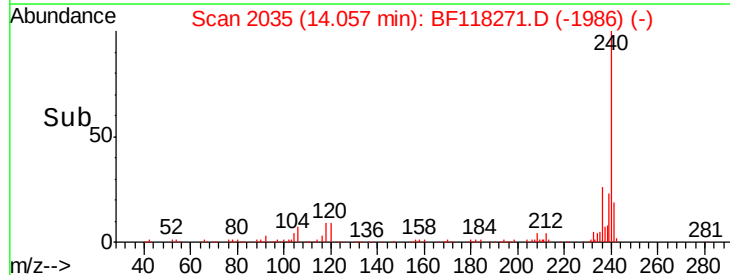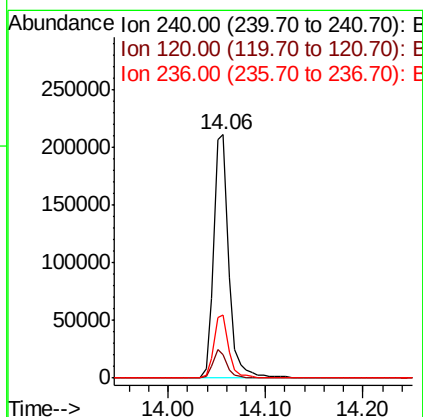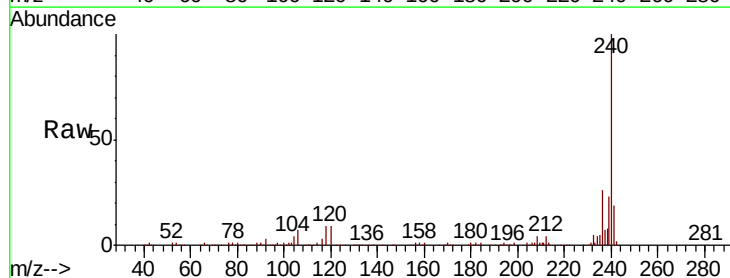

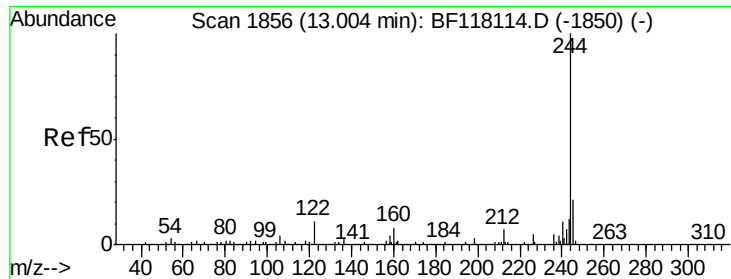

#79

Terphenyl-d14

Concen: 97.800 ng

RT: 12.99 min Scan# 1854

Delta R.T. -0.01 min

Lab File: BF118271.D

Acq: 18 Dec 2019 20:58

Instrument :

BNA_F

ClientSampleId :

PF-03





Tot Ion:244 Resp: 1296470

Ion Ratio Lower Upper

244 100

212 6.9 5.9 8.9

122 11.7 9.0 13.6

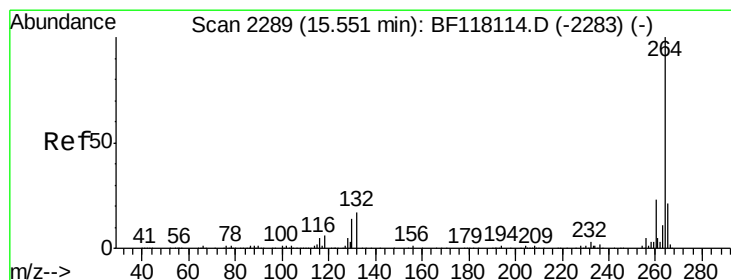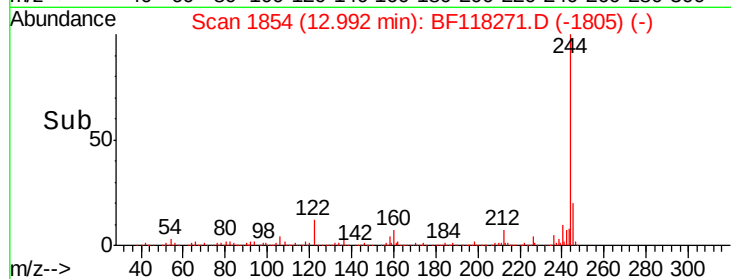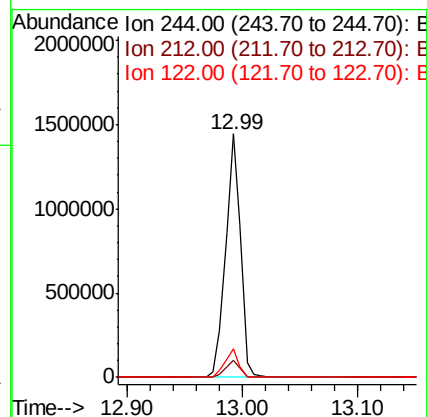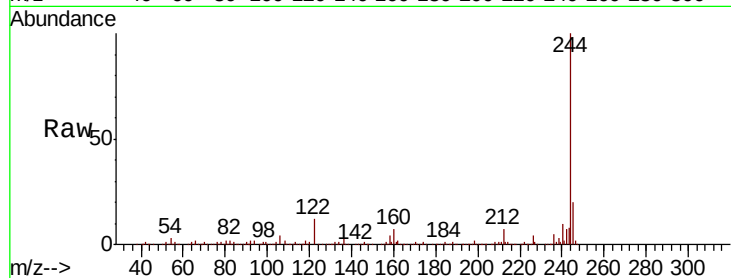

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.54 min Scan# 2288

Delta R.T. -0.01 min

Lab File: BF118271.D

Acq: 18 Dec 2019 20:58

Tgt Ion:264 Resp: 218291

Ion Ratio Lower Upper

264 100

260 24.8 18.6 28.0

265 21.9 16.8 25.2

