
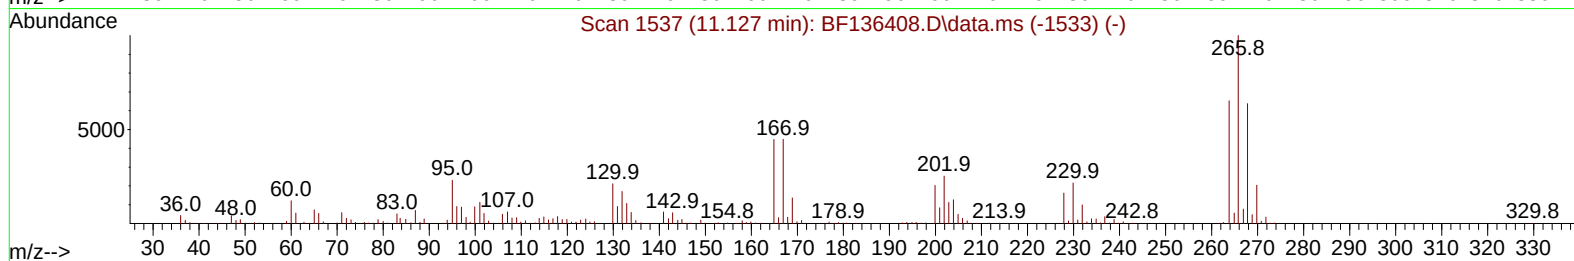
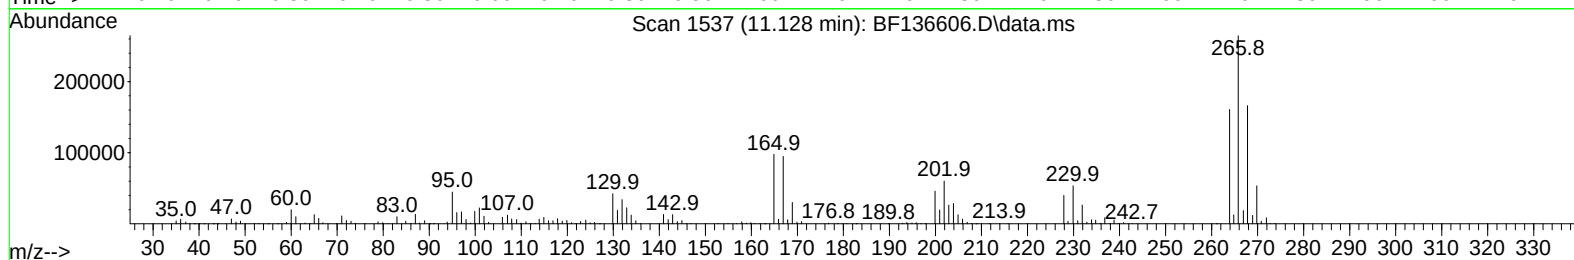


Quant Time: Dec 18 12:19:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 15 00:33:23 2023
Response via : Initial Calibration

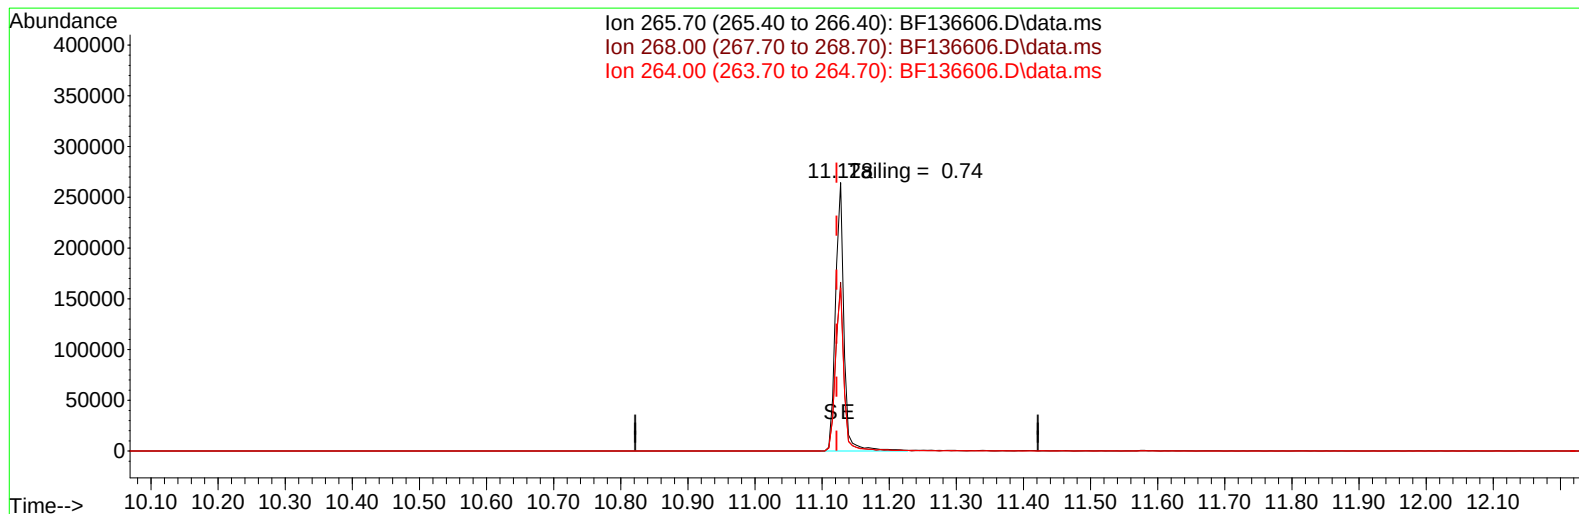

TIC: BF136606.D\data.ms

11.128min (+ 0.006) 27832.70 ng

response **230081**

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------




268.00	63.80	62.85
--------	-------	-------

264.00	65.30	60.77
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136606.D
Acq On : 18 Dec 2023 10:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 18 12:19:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 15 00:33:23 2023
Response via : Initial Calibration

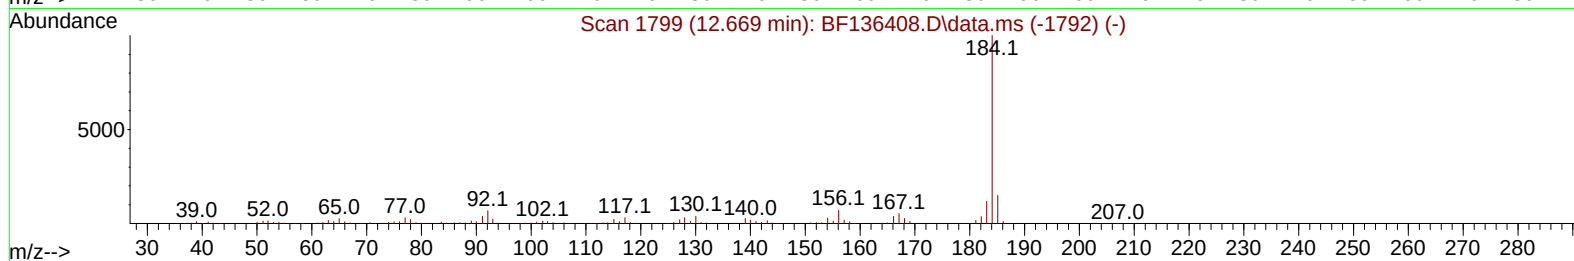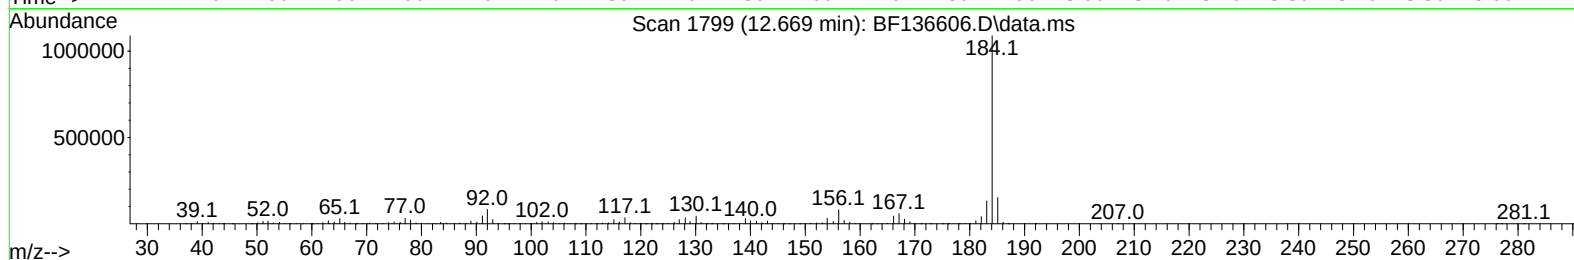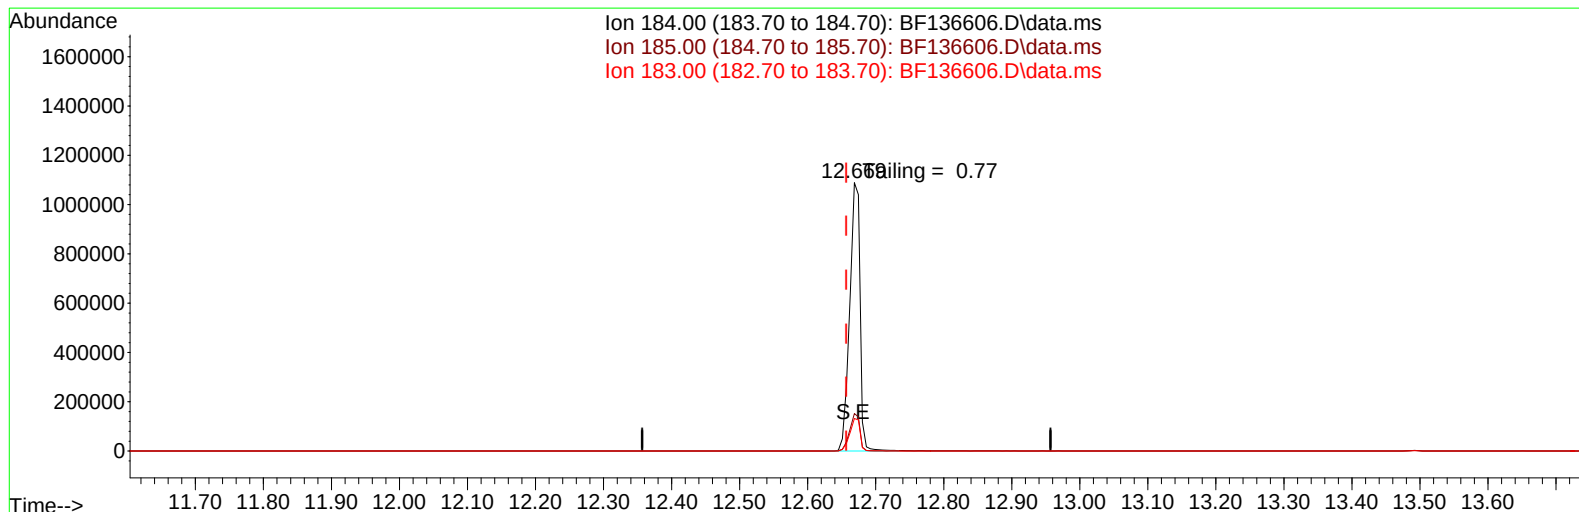

TIC: BF136606.D\data.ms

(77) Benzidine

12.669min (+ 0.012) 3426.20 ng m

response 1150963

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.94
183.00	11.70	12.14
0.00	0.00	0.00