

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136611.D
Acq On : 18 Dec 2023 13:21
Operator : CG\JU
Sample : PB157801BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157801BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136611.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.051	500	504	511	rVB	47409	65002	1.44%	0.261%
2	5.439	565	570	573	rBV	3139922	3003747	66.41%	12.058%
3	6.439	734	740	743	rBV	2716711	2984244	65.98%	11.980%
4	6.786	795	799	802	rBV	869888	662919	14.66%	2.661%
5	7.351	889	895	898	rBV	1965384	2012945	44.51%	8.081%
6	8.063	1011	1016	1020	rBV	1094216	941817	20.82%	3.781%
7	9.145	1194	1200	1203	rBV	4430574	4299220	95.06%	17.259%
8	9.822	1310	1315	1319	rBV	1373841	1140895	25.23%	4.580%
9	10.621	1446	1451	1454	rBV	2674930	2482340	54.89%	9.965%
10	11.316	1565	1569	1572	rBV	1476441	1190768	26.33%	4.780%
11	12.733	1806	1810	1813	rBV	77444	62444	1.38%	0.251%
12	12.915	1836	1841	1844	rBV	4685155	4522723	100.00%	18.156%
13	13.968	2016	2020	2027	rBV	915139	837847	18.53%	3.364%
14	15.451	2266	2272	2278	rBV	549872	702879	15.54%	2.822%




Sum of corrected areas: 24909790

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136611.D
Acq On : 18 Dec 2023 13:21
Operator : CG\JU
Sample : PB157801BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157801BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

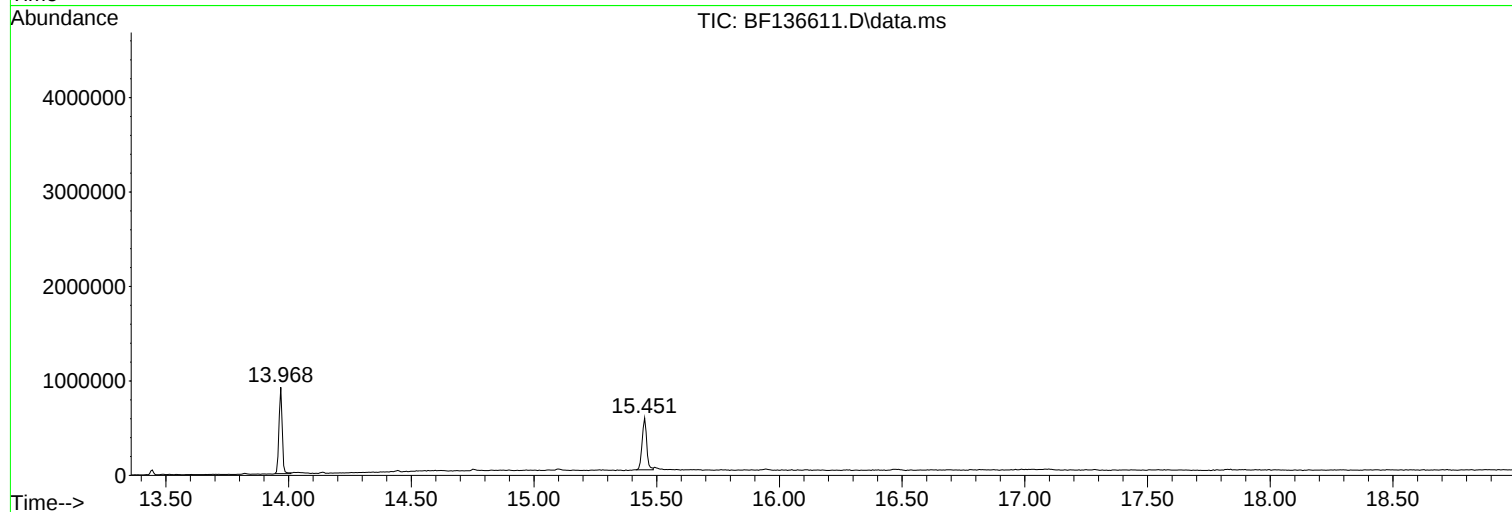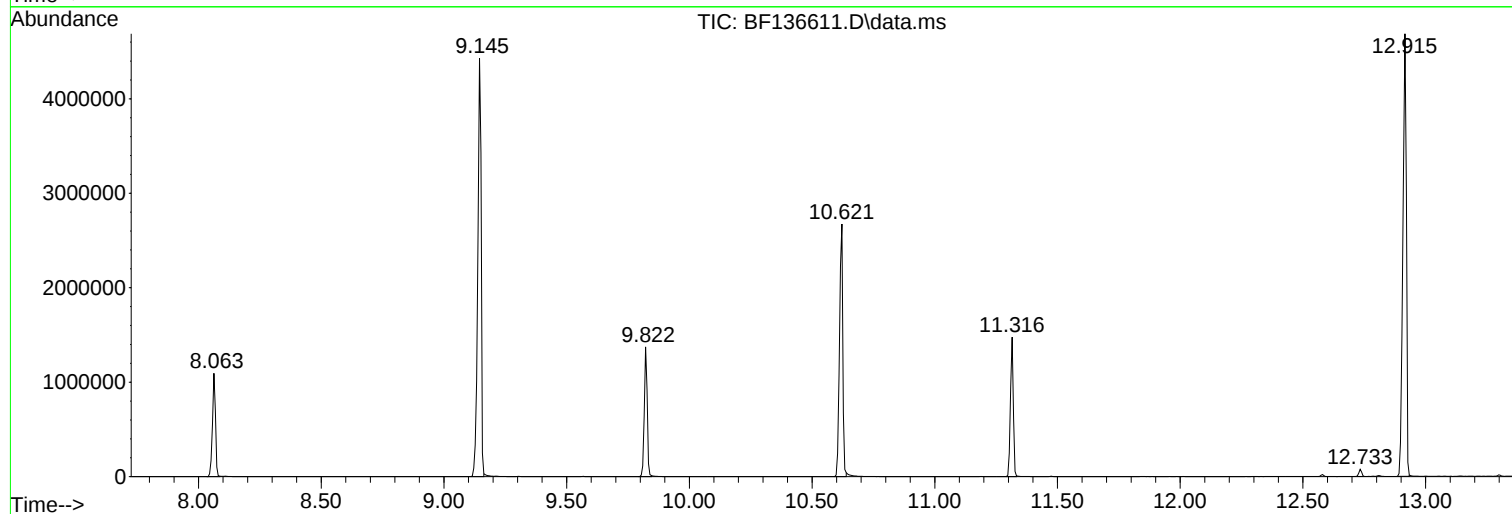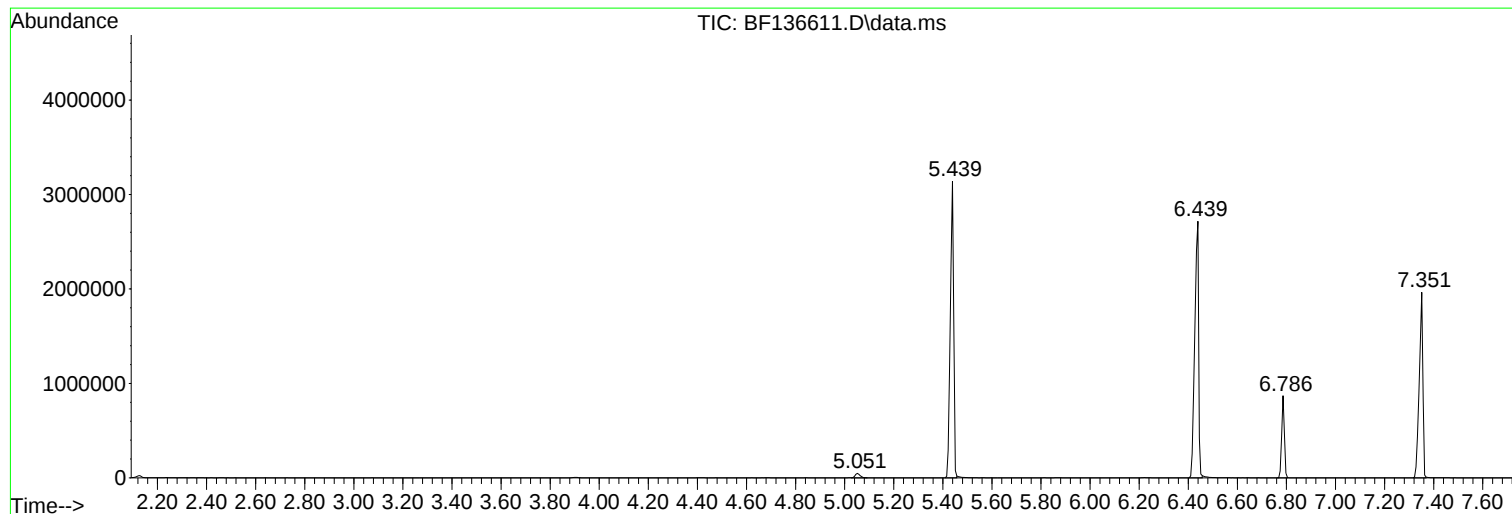

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136611.D
Acq On : 18 Dec 2023 13:21
Operator : CG\JU
Sample : PB157801BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157801BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136611.D
Acq On : 18 Dec 2023 13:21
Operator : CG\JU
Sample : PB157801BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157801BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------