

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
 Data File : BF136622.D
 Acq On : 18 Dec 2023 19:10
 Operator : CG\JU
 Sample : 05699-01RE
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ELM-N7THSTREET-DRUMS-SOILRE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136622.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.169	10	14	21	rVB2	23056	36878	2.38%	0.301%
2	5.016	494	498	507	rVB	327410	358680	23.15%	2.932%
3	5.428	564	568	582	rBV	1608273	1476691	95.30%	12.070%
4	6.434	734	739	742	rBV	1577048	1369139	88.35%	11.191%
5	6.787	796	799	803	rBV	670157	500907	32.33%	4.094%
6	7.345	890	894	897	rBV	1017771	900052	58.08%	7.357%
7	8.063	1012	1016	1020	rBV	789779	615201	39.70%	5.028%
8	9.139	1196	1199	1203	rBV	1757625	1549594	100.00%	12.666%
9	9.822	1311	1315	1319	rBV	740693	582828	37.61%	4.764%
10	10.616	1446	1450	1461	rBV	773546	744949	48.07%	6.089%
11	11.310	1565	1568	1571	rBV	602332	544997	35.17%	4.455%
12	11.333	1571	1572	1577	rVV	69374	55356	3.57%	0.452%
13	11.386	1577	1581	1585	rVB2	17597	20213	1.30%	0.165%
14	11.845	1656	1659	1664	rBV	116081	118883	7.67%	0.972%
15	11.928	1670	1673	1676	rBV2	16094	20638	1.33%	0.169%
16	12.104	1700	1703	1707	rBV3	14385	20993	1.35%	0.172%
17	12.533	1772	1776	1780	rBV	129216	123663	7.98%	1.011%
18	12.639	1789	1794	1797	rBV5	34187	45859	2.96%	0.375%
19	12.763	1807	1815	1818	rBV2	118977	144173	9.30%	1.178%
20	12.910	1836	1840	1843	rBV	1834924	1480080	95.51%	12.098%
21	12.975	1849	1851	1857	rVB4	12203	21815	1.41%	0.178%
22	13.192	1885	1888	1891	rBV2	27004	31510	2.03%	0.258%
23	13.604	1955	1958	1963	rBV	26125	33766	2.18%	0.276%
24	13.822	1991	1995	1999	rVB2	37329	42065	2.71%	0.344%
25	13.969	2015	2020	2023	rBV	740882	702032	45.30%	5.738%
26	13.992	2023	2024	2026	rVB	75789	43060	2.78%	0.352%
27	14.604	2125	2128	2132	rBV2	64563	62765	4.05%	0.513%
28	15.016	2195	2198	2200	rBV	56887	66937	4.32%	0.547%
29	15.380	2258	2260	2266	rBV	40820	52661	3.40%	0.430%
30	15.451	2267	2272	2276	rBV	386089	468021	30.20%	3.825%




Sum of corrected areas: 12234406

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136622.D
Acq On : 18 Dec 2023 19:10
Operator : CG\JU
Sample : 05699-01RE
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ELM-N7THSTREET-DRUMS-SOILRE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

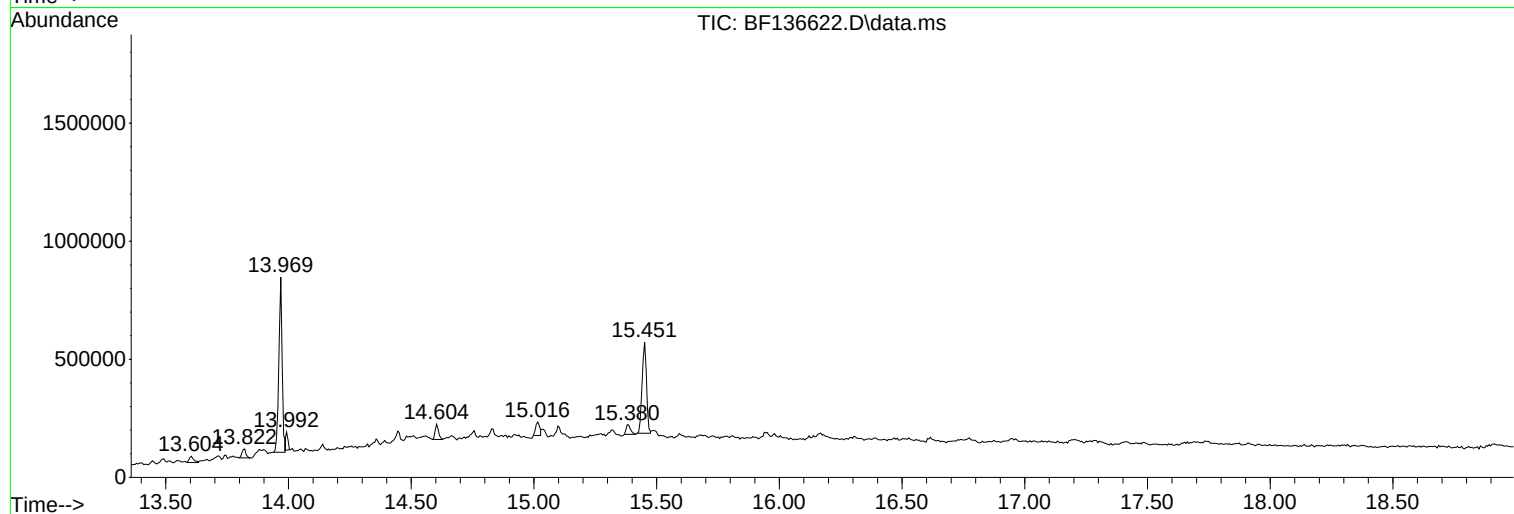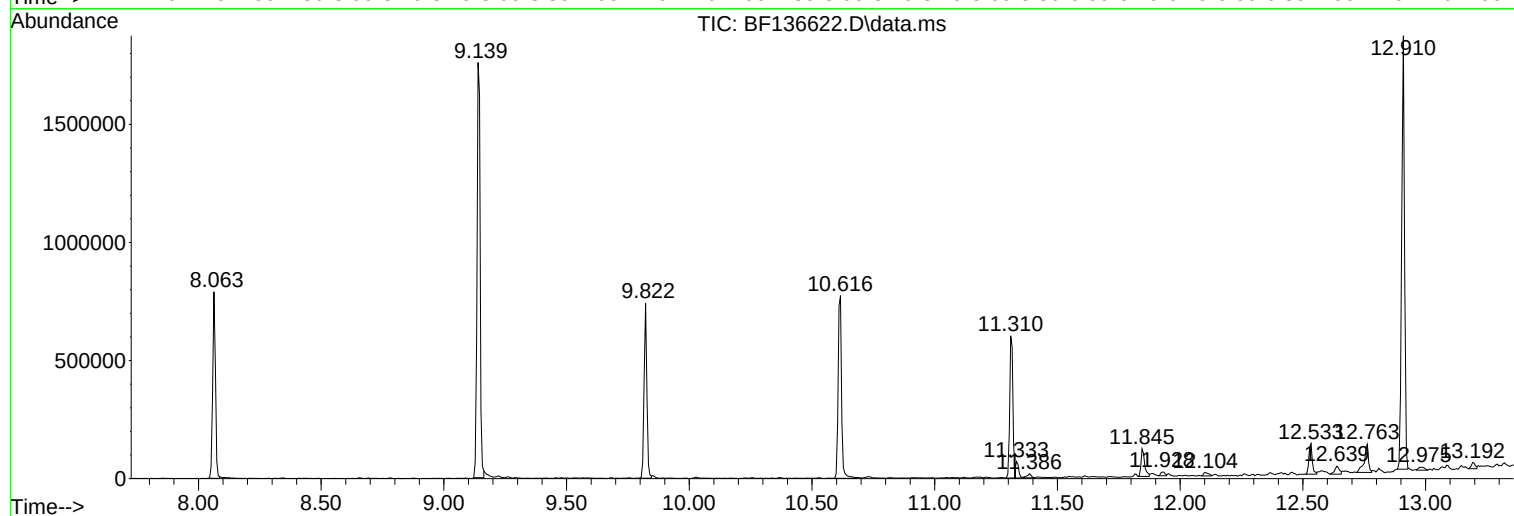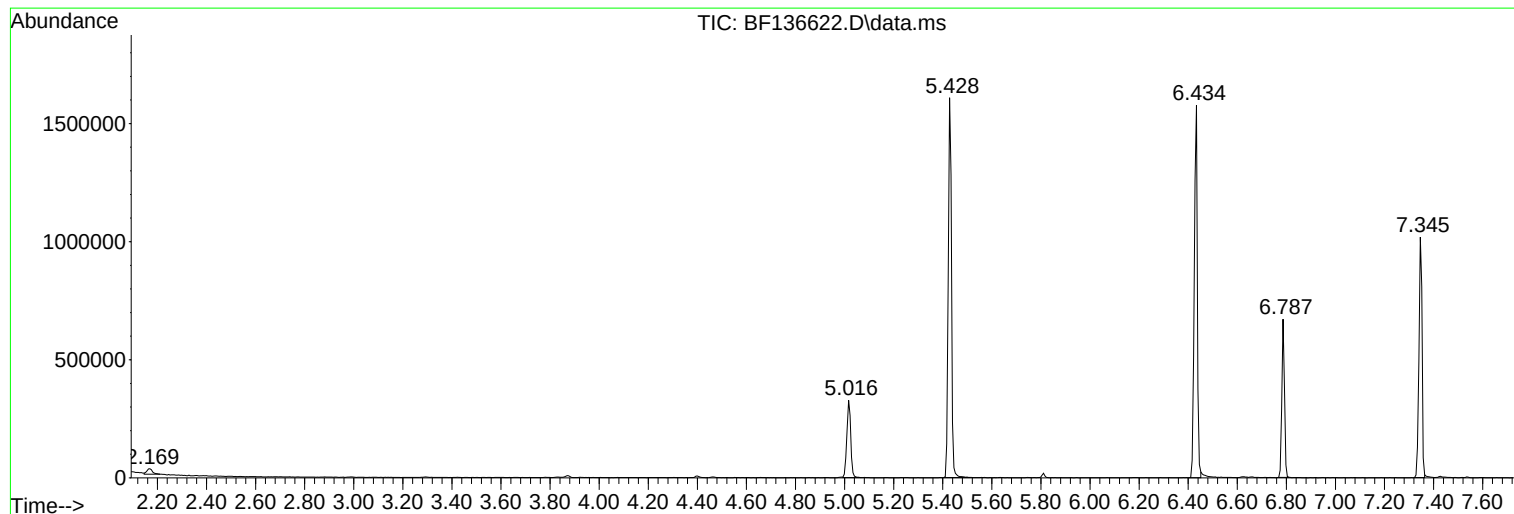

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136622.D
Acq On : 18 Dec 2023 19:10
Operator : CG\JU
Sample : 05699-01RE
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ELM-N7THSTREET-DRUMS-SOILRE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136622.D
Acq On : 18 Dec 2023 19:10
Operator : CG\JU
Sample : 05699-01RE
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ELM-N7THSTREET-DRUMS-SOILRE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------