

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
 Data File : BF136624.D
 Acq On : 18 Dec 2023 20:14
 Operator : CG\JU
 Sample : 05767-04RE
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP-E2-COMPRES

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136624.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.151	8	11	19	rVB4	12104	19803	1.29%	0.158%
2	5.016	494	498	504	rVB	29516	35253	2.29%	0.282%
3	5.428	564	568	580	rBV	1524814	1337580	87.00%	10.681%
4	6.434	735	739	747	rBV	1440338	1221586	79.46%	9.755%
5	6.786	796	799	803	rBV	549214	432549	28.13%	3.454%
6	7.345	890	894	897	rBV	917416	777071	50.54%	6.205%
7	8.063	1011	1016	1019	rBV	587587	495189	32.21%	3.954%
8	9.145	1196	1200	1203	rBV	1562175	1323067	86.06%	10.566%
9	9.669	1286	1289	1297	rBV2	37575	56714	3.69%	0.453%
10	9.822	1312	1315	1318	rBV	619537	463622	30.16%	3.702%
11	10.616	1446	1450	1459	rBV	863504	755851	49.16%	6.036%
12	10.739	1467	1471	1477	rVB5	13868	20565	1.34%	0.164%
13	11.316	1565	1569	1571	rBV	643406	521408	33.91%	4.164%
14	11.339	1571	1573	1577	rVV	130290	111230	7.23%	0.888%
15	11.386	1577	1581	1585	rVB	42318	50075	3.26%	0.400%
16	11.816	1651	1654	1656	rBV	23471	19430	1.26%	0.155%
17	11.851	1656	1660	1665	rBV	228613	225185	14.65%	1.798%
18	11.927	1670	1673	1676	rBV	40621	46182	3.00%	0.369%
19	12.010	1684	1687	1692	rBV5	15589	27245	1.77%	0.218%
20	12.145	1707	1710	1713	rVB4	17367	19597	1.27%	0.156%
21	12.368	1745	1748	1751	rBV2	27792	28678	1.87%	0.229%
22	12.457	1760	1763	1768	rVB4	22921	26449	1.72%	0.211%
23	12.533	1772	1776	1779	rBV	377238	320648	20.86%	2.561%
24	12.574	1779	1783	1786	rVV6	20287	30772	2.00%	0.246%
25	12.639	1790	1794	1798	rBV2	78655	91122	5.93%	0.728%
26	12.763	1808	1815	1818	rBV	356206	345118	22.45%	2.756%
27	12.910	1836	1840	1843	rBV	1937734	1537438	100.00%	12.277%
28	12.980	1849	1852	1856	rBV3	26026	41577	2.70%	0.332%
29	13.092	1868	1871	1875	rVB	62532	64285	4.18%	0.513%
30	13.157	1880	1882	1885	rVB	33716	32073	2.09%	0.256%
31	13.198	1886	1889	1892	rBV2	42170	42449	2.76%	0.339%
32	13.292	1903	1905	1907	rBV	24270	20325	1.32%	0.162%
33	13.604	1956	1958	1963	rVB	50805	53685	3.49%	0.429%
34	13.745	1980	1982	1983	rBV	32125	21989	1.43%	0.176%
35	13.768	1983	1986	1992	rVV2	70563	94000	6.11%	0.751%
36	13.815	1992	1994	1998	rVB2	35646	38417	2.50%	0.307%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136624.D
Acq On : 18 Dec 2023 20:14
Operator : CG\JU
Sample : 05767-04RE
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-E2-COMPRE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	13.968	2015	2020	2023	rBV2	695124	807084	52.50%	6.445%
38	13.992	2023	2024	2031	rVB	188161	167063	10.87%	1.334%
39	15.015	2194	2198	2201	rBV	167995	256541	16.69%	2.049%
40	15.386	2258	2261	2267	rVB	134796	160443	10.44%	1.281%
41	15.451	2268	2272	2276	rBV	290611	383045	24.91%	3.059%




Sum of corrected areas: 12522403

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136624.D
Acq On : 18 Dec 2023 20:14
Operator : CG\JU
Sample : 05767-04RE
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-E2-COMPTE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

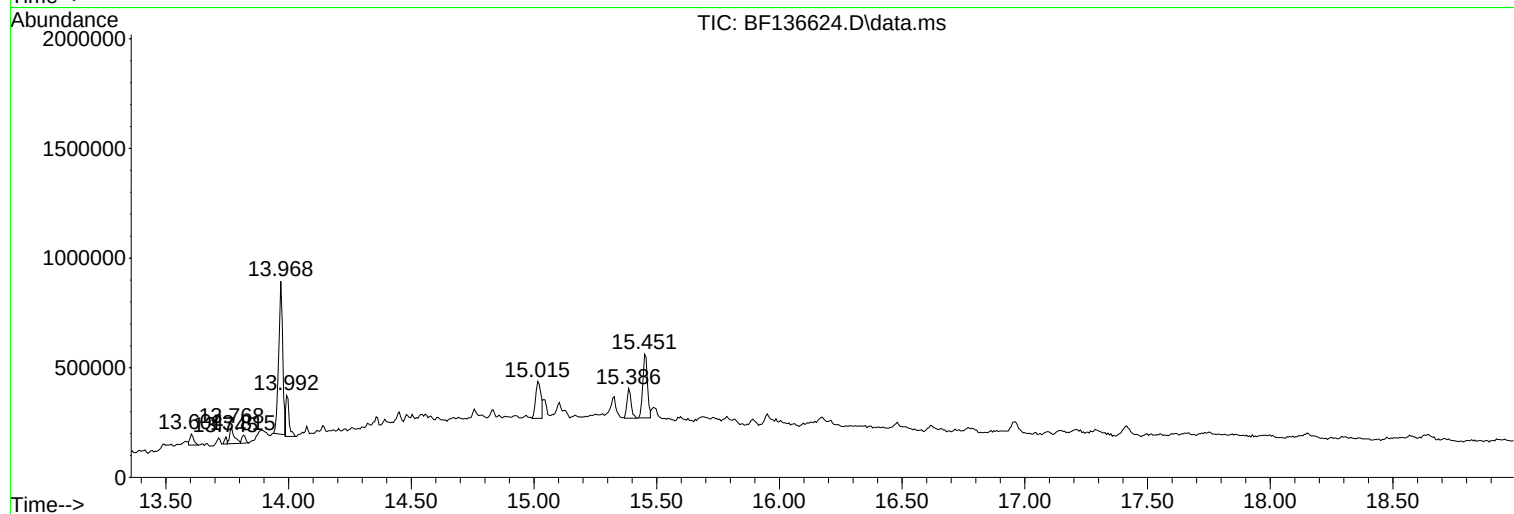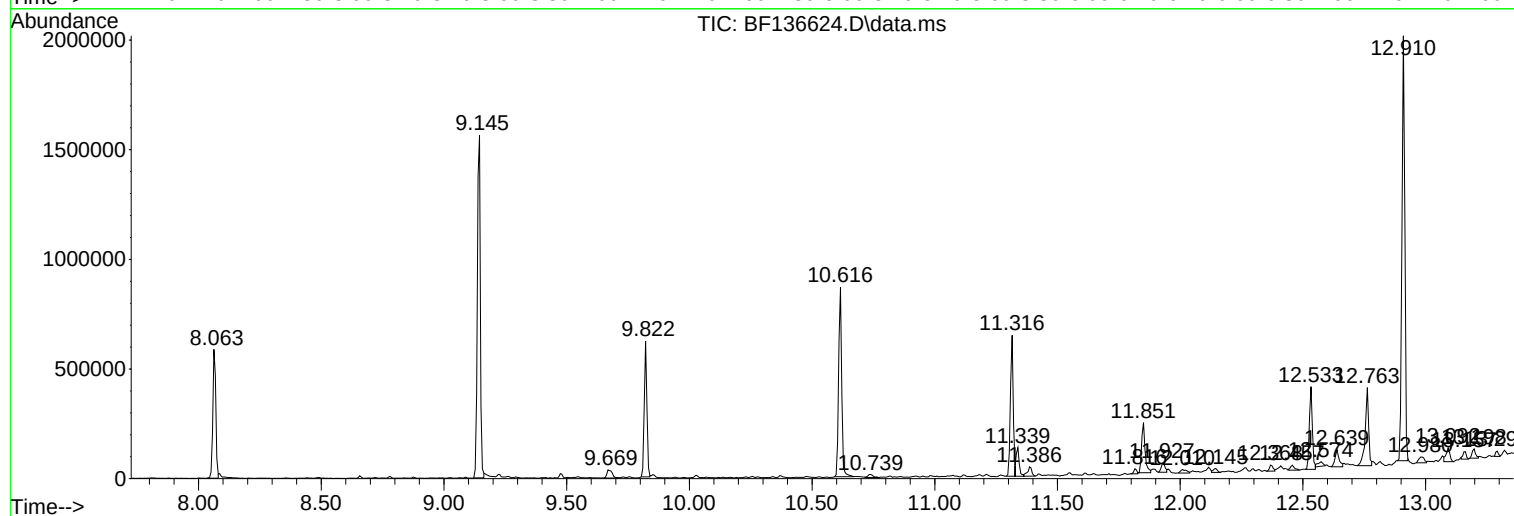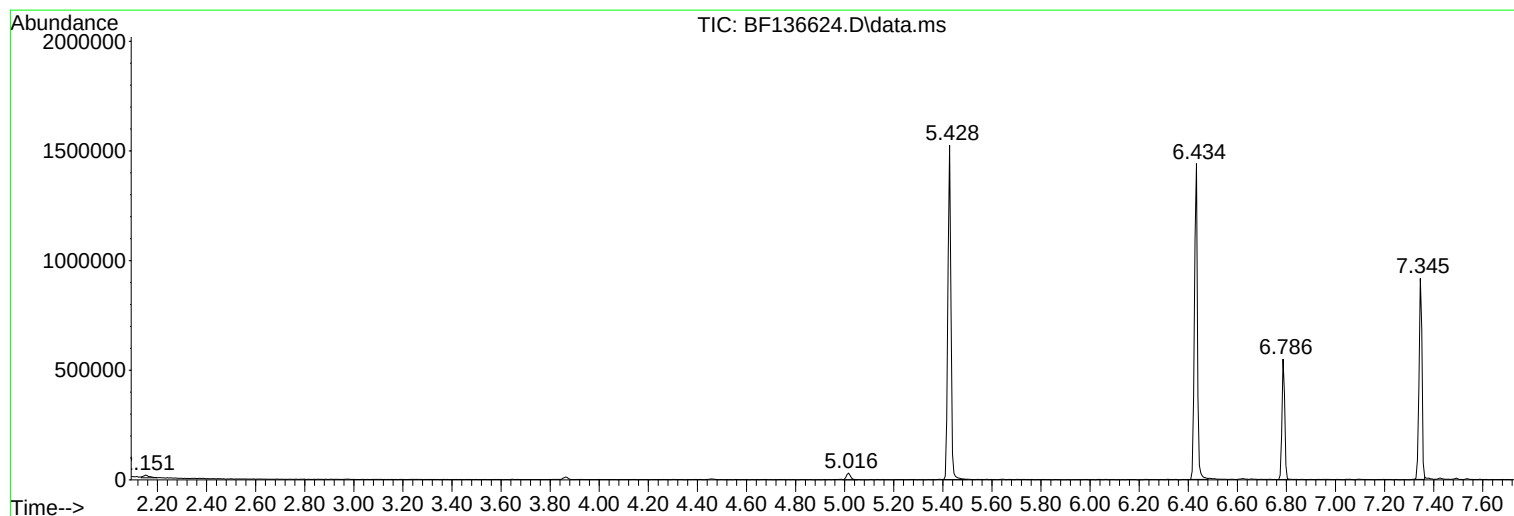

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136624.D
Acq On : 18 Dec 2023 20:14
Operator : CG\JU
Sample : 05767-04RE
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-E2-COMPRE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136624.D
Acq On : 18 Dec 2023 20:14
Operator : CG\JU
Sample : 05767-04RE
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-E2-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------