

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
 Data File : BF136625.D
 Acq On : 18 Dec 2023 20:45
 Operator : CG\JU
 Sample : 05726-01RE
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-1RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136625.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.022	495	499	505	rVB	34637	39787	2.38%	0.171%
2	5.434	564	569	572	rBV	1581401	1536254	91.75%	6.607%
3	6.434	735	739	742	rBV	1645549	1376415	82.20%	5.920%
4	6.787	796	799	803	rBV	537316	409174	24.44%	1.760%
5	7.345	890	894	897	rBV	993008	893842	53.38%	3.844%
6	8.063	1012	1016	1019	rBV	607955	477808	28.54%	2.055%
7	9.145	1196	1200	1203	rBV	1627158	1421020	84.87%	6.112%
8	9.545	1263	1268	1273	rVB	22308	21682	1.29%	0.093%
9	9.681	1289	1291	1295	rBV	85076	71678	4.28%	0.308%
10	9.822	1311	1315	1318	rBV	594533	461159	27.54%	1.983%
11	9.851	1318	1320	1325	rVB	35767	32535	1.94%	0.140%
12	10.028	1346	1350	1354	rBV	32805	30974	1.85%	0.133%
13	10.369	1405	1408	1415	rVB	44670	49999	2.99%	0.215%
14	10.616	1446	1450	1463	rVB	1108139	938313	56.04%	4.036%
15	10.739	1466	1471	1475	rBV3	44378	64222	3.84%	0.276%
16	10.922	1497	1502	1504	rBV2	25734	29076	1.74%	0.125%
17	11.069	1521	1527	1530	rVB4	19160	30386	1.81%	0.131%
18	11.181	1544	1546	1549	rVV3	36170	29061	1.74%	0.125%
19	11.210	1549	1551	1555	rVB	53373	48030	2.87%	0.207%
20	11.316	1565	1569	1571	rBV	617633	550857	32.90%	2.369%
21	11.339	1571	1573	1576	rVV	433823	333603	19.92%	1.435%
22	11.392	1578	1582	1585	rVV	170174	163631	9.77%	0.704%
23	11.422	1585	1587	1591	rVB	72826	65121	3.89%	0.280%
24	11.469	1592	1595	1598	rVV	75716	68836	4.11%	0.296%
25	11.551	1605	1609	1611	rBV2	30916	32647	1.95%	0.140%
26	11.616	1617	1620	1622	rVB2	36164	30255	1.81%	0.130%
27	11.645	1623	1625	1630	rVB2	25049	31337	1.87%	0.135%
28	11.728	1637	1639	1643	rVB3	36082	35858	2.14%	0.154%
29	11.769	1643	1646	1651	rBV4	30838	40292	2.41%	0.173%
30	11.816	1651	1654	1657	rBV	89265	89924	5.37%	0.387%
31	11.851	1657	1660	1665	rBV2	346275	317795	18.98%	1.367%
32	11.892	1665	1667	1670	rBV	49237	39459	2.36%	0.170%
33	11.933	1670	1674	1676	rBV2	278499	263274	15.72%	1.132%
34	12.051	1691	1694	1696	rBV4	31393	25942	1.55%	0.112%
35	12.116	1700	1705	1707	rVV	78329	94178	5.62%	0.405%
36	12.145	1707	1710	1714	rVB2	61510	59113	3.53%	0.254%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
 Data File : BF136625.D
 Acq On : 18 Dec 2023 20:45
 Operator : CG\JU
 Sample : 05726-01RE
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-1RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	12.263	1725	1730	1733	rBV4	52912	65801	3.93%	0.283%
38	12.298	1733	1736	1738	rVV2	36288	38719	2.31%	0.167%
39	12.322	1738	1740	1742	rVB	33094	26128	1.56%	0.112%
40	12.375	1745	1749	1751	rBV	93557	106037	6.33%	0.456%
41	12.410	1751	1755	1757	rVV2	72907	86048	5.14%	0.370%
42	12.427	1757	1758	1761	rVV	33071	25545	1.53%	0.110%
43	12.457	1761	1763	1767	rVV2	65974	71224	4.25%	0.306%
44	12.492	1767	1769	1772	rVB3	24513	22125	1.32%	0.095%
45	12.539	1772	1777	1780	rBV	1429915	1353512	80.83%	5.821%
46	12.580	1780	1784	1786	rVV2	57292	66188	3.95%	0.285%
47	12.639	1790	1794	1799	rBV2	89923	143881	8.59%	0.619%
48	12.686	1799	1802	1806	rVV2	57724	76639	4.58%	0.330%
49	12.769	1809	1816	1819	rVV	1347351	1417719	84.67%	6.098%
50	12.816	1821	1824	1829	rVB2	62362	86448	5.16%	0.372%
51	12.880	1832	1835	1837	rBV2	78233	84853	5.07%	0.365%
52	12.910	1837	1840	1847	rVB	1823268	1674440	100.00%	7.202%
53	12.986	1848	1853	1857	rBV4	119466	199803	11.93%	0.859%
54	13.045	1860	1863	1865	rVV2	89928	84691	5.06%	0.364%
55	13.069	1865	1867	1869	rVV3	96772	121251	7.24%	0.521%
56	13.098	1869	1872	1875	rVB	231886	233634	13.95%	1.005%
57	13.163	1880	1883	1885	rVB	203963	160447	9.58%	0.690%
58	13.198	1885	1889	1893	rBV2	186706	199975	11.94%	0.860%
59	13.257	1897	1899	1902	rBV3	38071	38178	2.28%	0.164%
60	13.292	1902	1905	1908	rBV	117608	92289	5.51%	0.397%
61	13.322	1908	1910	1913	rBV	109999	94628	5.65%	0.407%
62	13.580	1951	1954	1956	rBV4	58498	67928	4.06%	0.292%
63	13.604	1956	1958	1963	rVB	103184	128155	7.65%	0.551%
64	13.716	1974	1977	1980	rBV2	127229	123765	7.39%	0.532%
65	13.745	1980	1982	1984	rVV	111233	86391	5.16%	0.372%
66	13.769	1984	1986	1992	rVV3	113581	147060	8.78%	0.633%
67	13.816	1992	1994	1998	rVB2	115094	105712	6.31%	0.455%
68	13.963	2015	2019	2023	rBV2	1006636	1467588	87.65%	6.312%
69	13.998	2023	2025	2031	rVB	763407	633229	37.82%	2.724%
70	14.074	2036	2038	2041	rVB	121192	109551	6.54%	0.471%
71	14.116	2043	2045	2047	rBV	51263	50743	3.03%	0.218%
72	14.321	2078	2080	2082	rBV	55160	53501	3.20%	0.230%
73	14.363	2084	2087	2090	rVV	164433	181284	10.83%	0.780%
74	14.392	2090	2092	2096	rVB	90966	84679	5.06%	0.364%
75	14.486	2105	2108	2110	rBV2	102439	95567	5.71%	0.411%
76	14.833	2164	2167	2169	rBV	72113	78694	4.70%	0.338%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136625.D
Acq On : 18 Dec 2023 20:45
Operator : CG\JU
Sample : 05726-01RE
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-1RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	15.021	2195	2199	2202	rBV	536517	795846	47.53%	3.423%
78	15.127	2215	2217	2221	rVB	123263	130798	7.81%	0.563%
79	15.327	2248	2251	2257	rVB	290820	375139	22.40%	1.613%
80	15.392	2258	2262	2268	rVV	440900	580846	34.69%	2.498%
81	15.457	2269	2273	2276	rVV	326053	419757	25.07%	1.805%
82	15.486	2276	2278	2287	rVB2	136863	212435	12.69%	0.914%
83	16.962	2524	2529	2537	rVB3	167960	343507	20.51%	1.477%
84	17.421	2603	2607	2613	rVB2	113556	204631	12.22%	0.880%




Sum of corrected areas: 23250546

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136625.D
Acq On : 18 Dec 2023 20:45
Operator : CG\JU
Sample : 05726-01RE
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-1RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

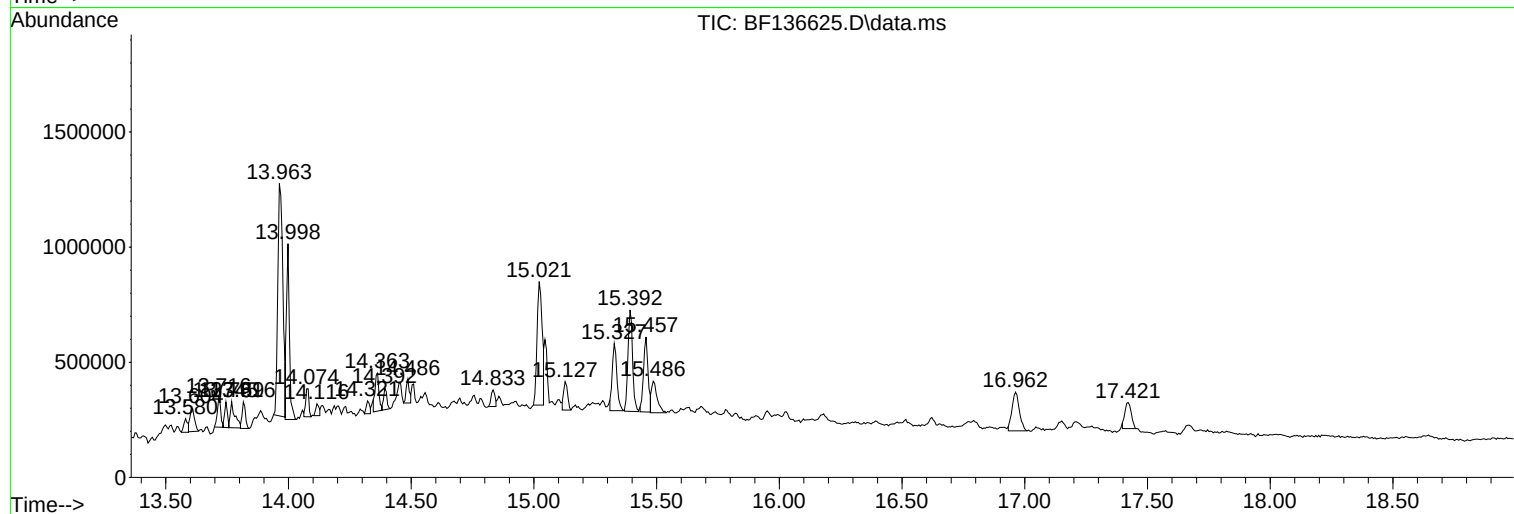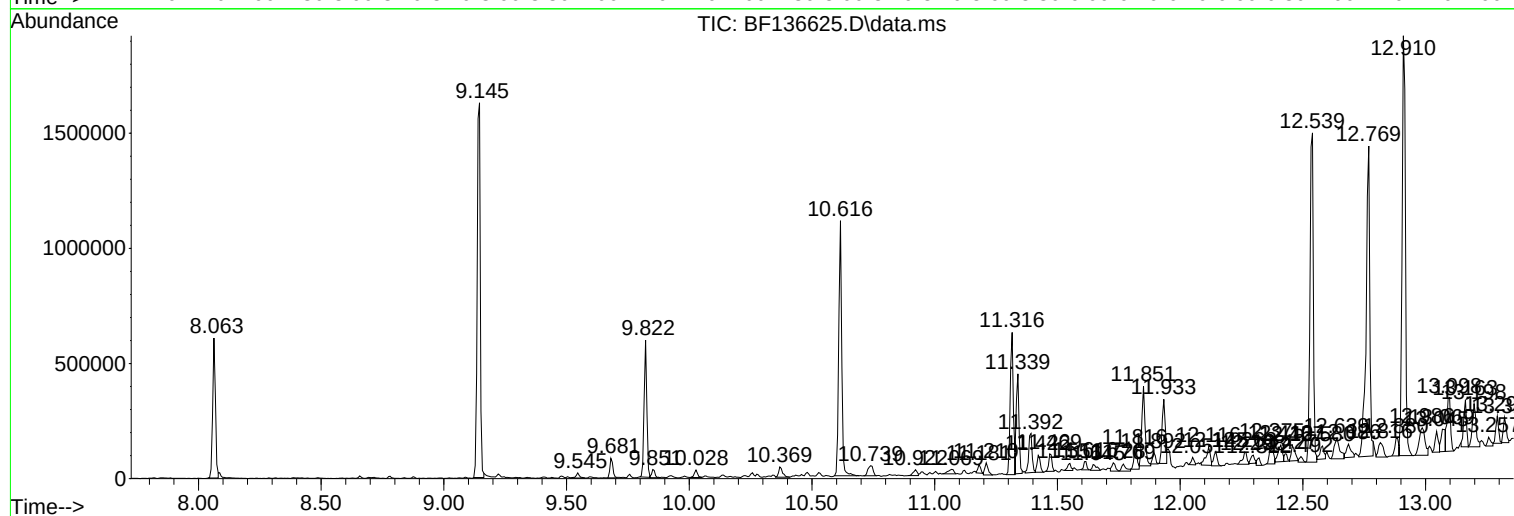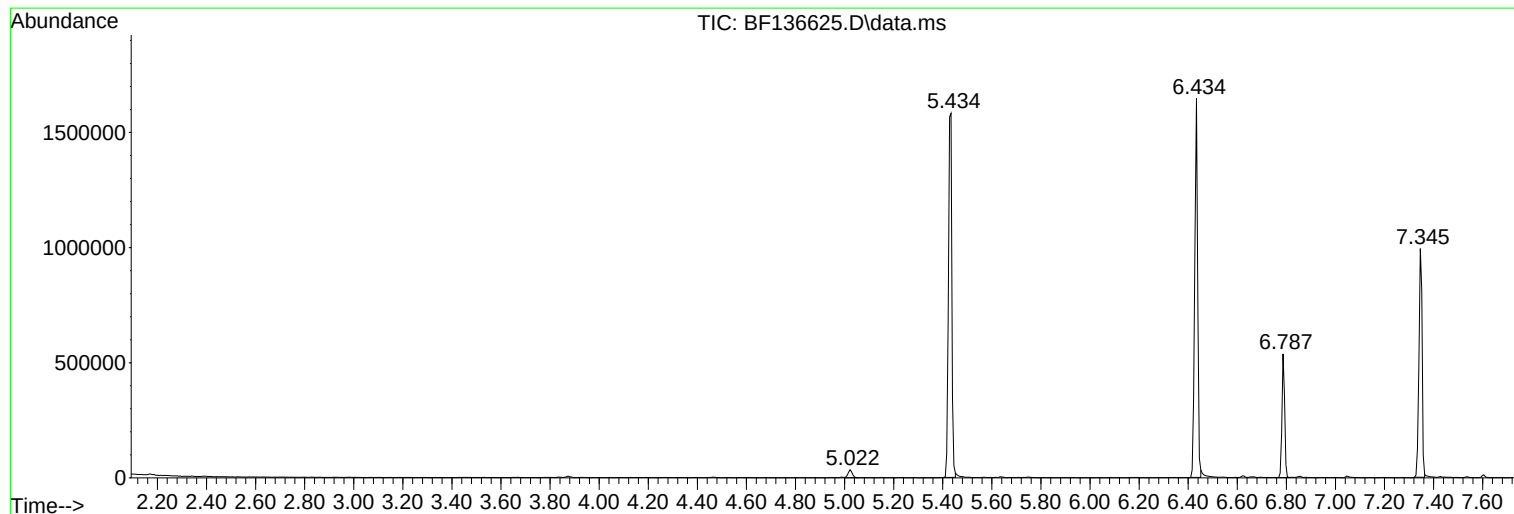

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136625.D
Acq On : 18 Dec 2023 20:45
Operator : CG\JU
Sample : 05726-01RE
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-1RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136625.D
Acq On : 18 Dec 2023 20:45
Operator : CG\JU
Sample : 05726-01RE
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-1RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------