
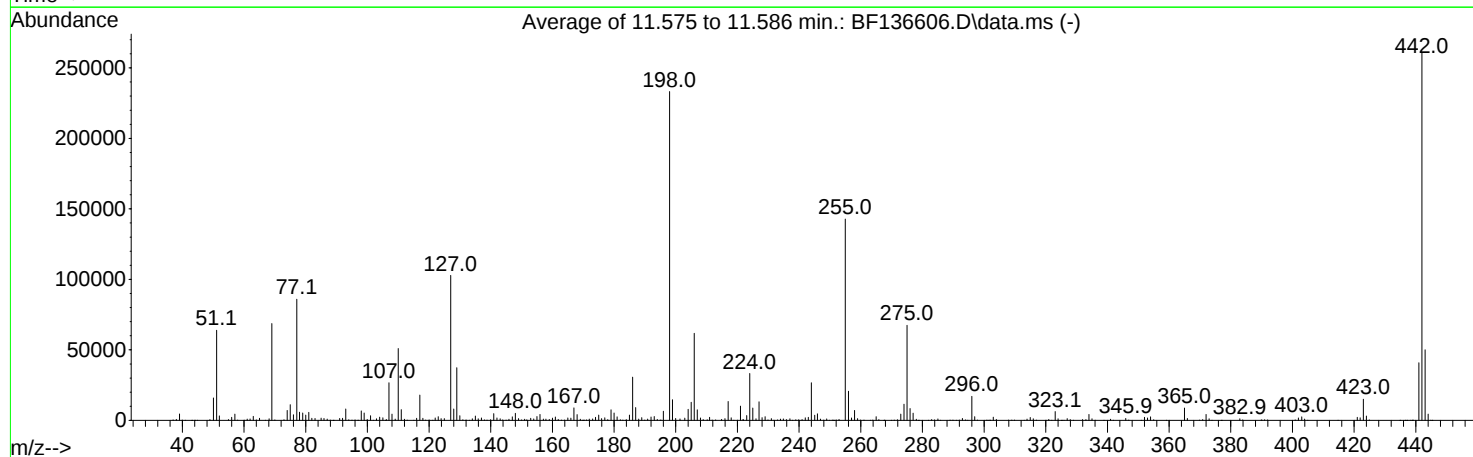


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136606.D
Acq On : 18 Dec 2023 10:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Dec 19 00:56:37 2023

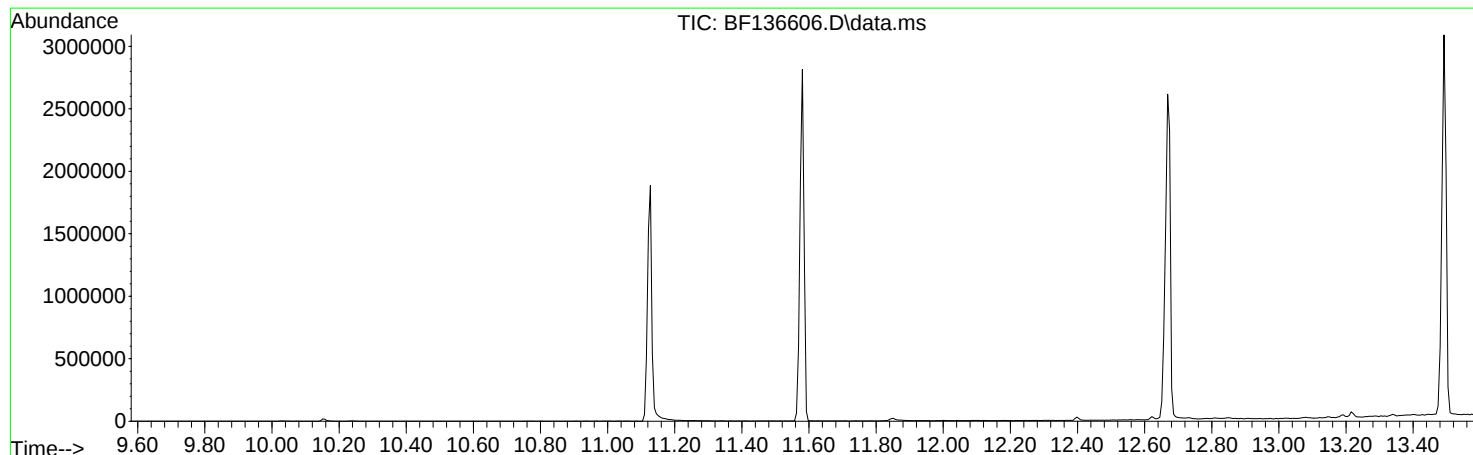




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	63960	PASS
68	69	0.00	2	1.6	1113	PASS
69	198	0.00	100	29.5	68680	PASS
70	69	0.00	2	0.6	396	PASS
127	198	10	80	44.1	102803	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	233187	PASS
199	198	5	9	6.3	14695	PASS
275	198	10	60	28.9	67480	PASS
365	198	1	100	3.8	8781	PASS
441	198	0.01	100	17.5	40845	PASS
442	442	50	100	100.0	260928	PASS
443	442	15	24	19.2	50037	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
 Data File : BF136606.D
 Acq On : 18 Dec 2023 10:44
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 18 12:19:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 15 00:33:23 2023
 Response via : Initial Calibration

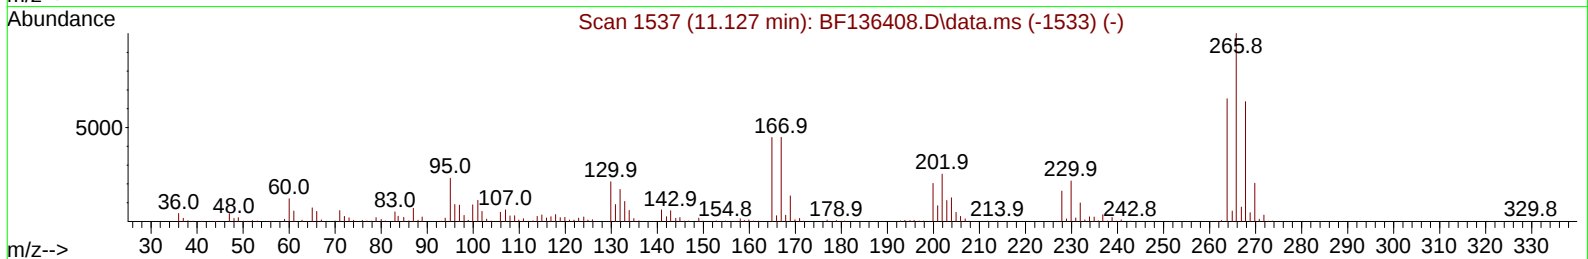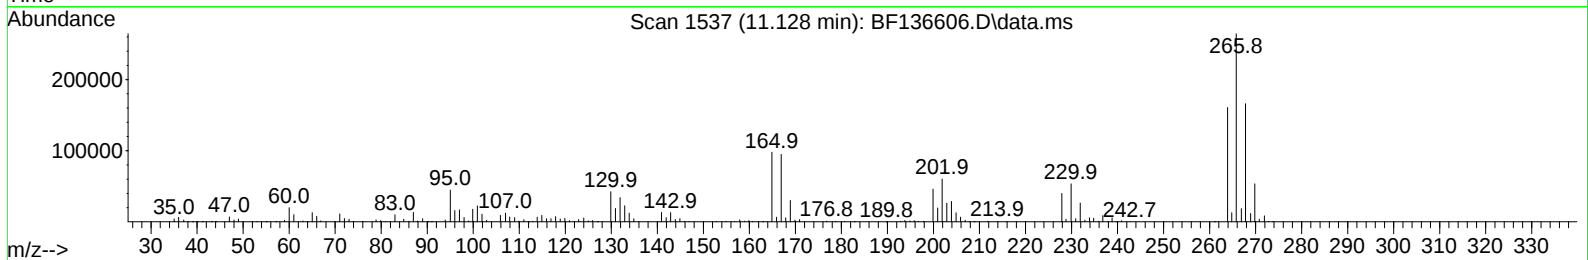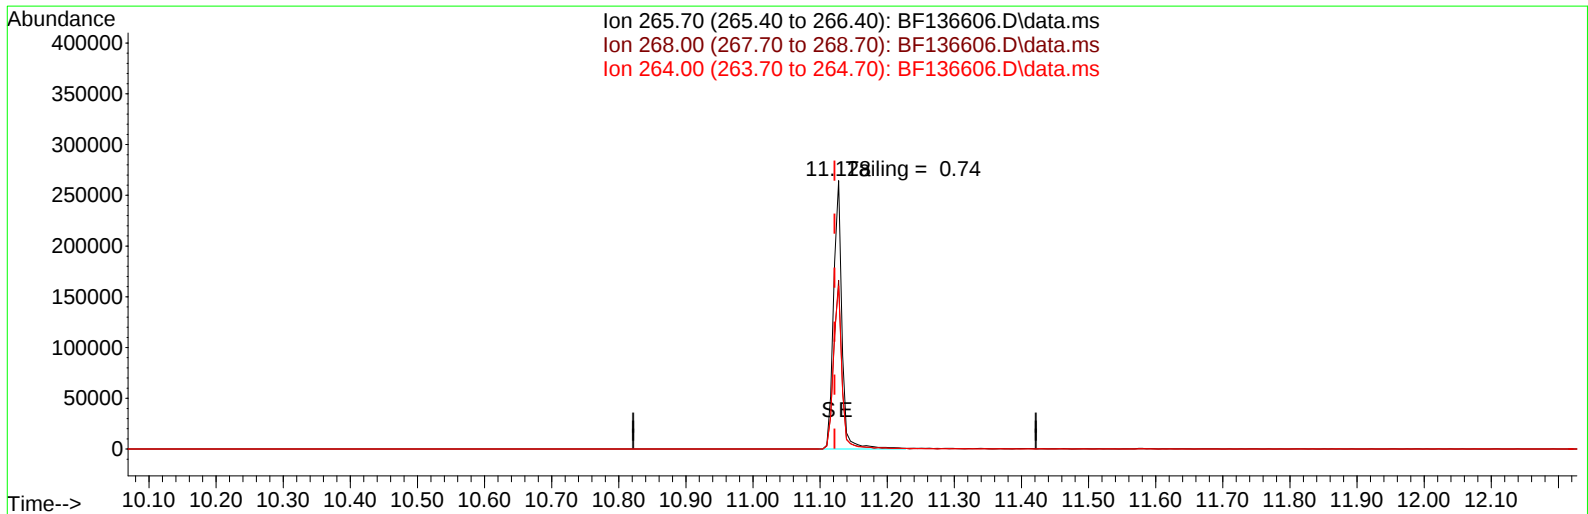

TIC: BF136606.D\data.ms

(70) Pentachlorophenol (C)

11.128min (+ 0.006) 27832.70 ng




response 230081

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.85
264.00	65.30	60.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121823\
Data File : BF136606.D
Acq On : 18 Dec 2023 10:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 18 12:19:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 15 00:33:23 2023
Response via : Initial Calibration

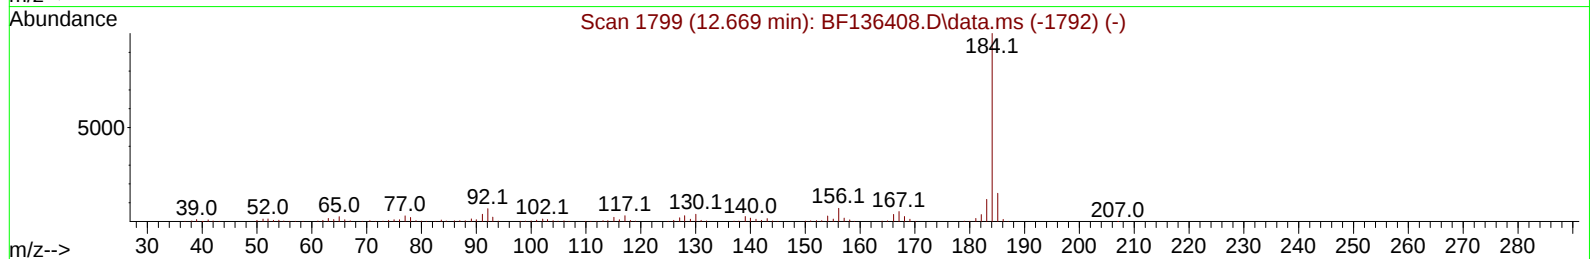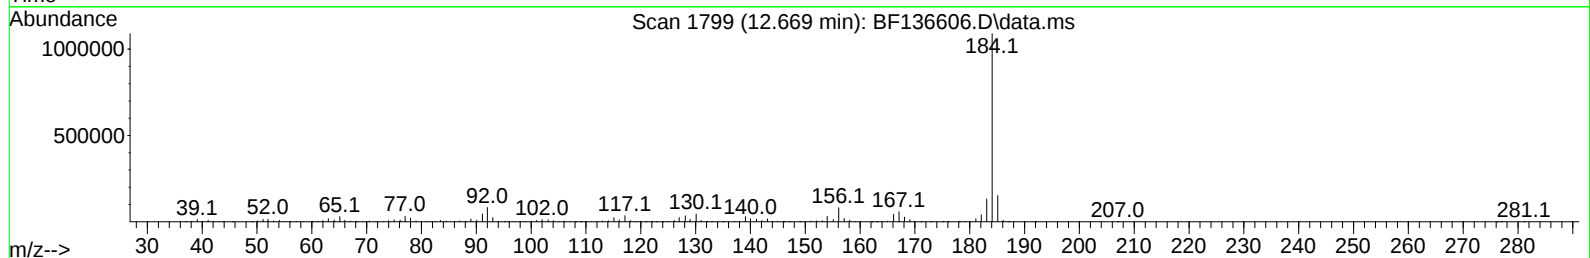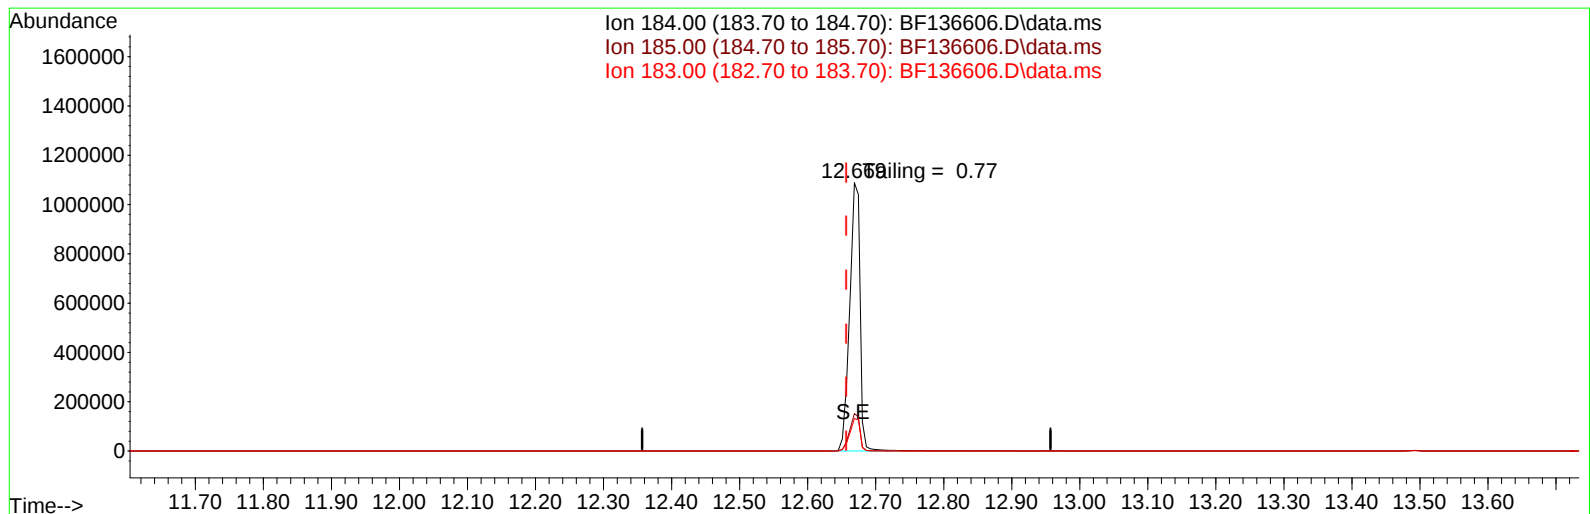

TIC: BF136606.D\data.ms

(77) Benzidine

12.669min (+ 0.012) 3426.20 ng m

response 1150963

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.94
183.00	11.70	12.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/18/2023	BNA_F	<u>BF136606.D</u>
Compound Name	Response	Retention Time
DDT	578313	13.492
DDD	11254	13.216
DDE	1304	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12558	590871	2.13

Instrument :
BNA_F
ClientSampleId :
DFTPP