
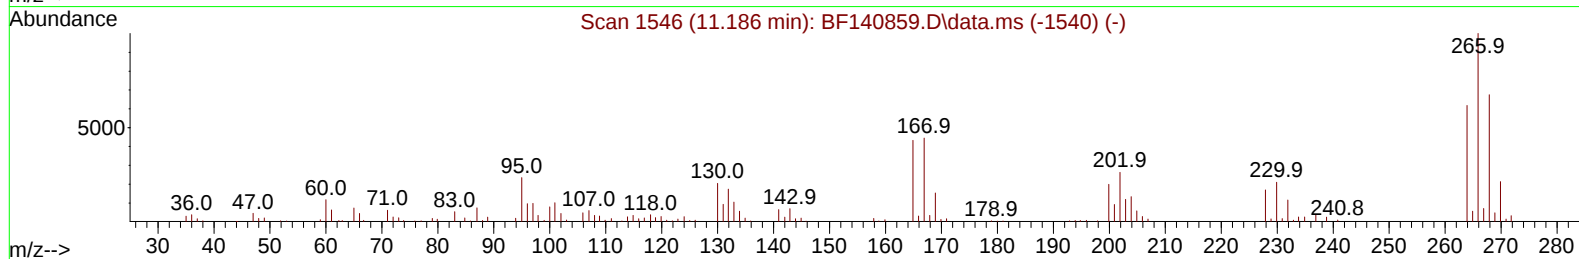
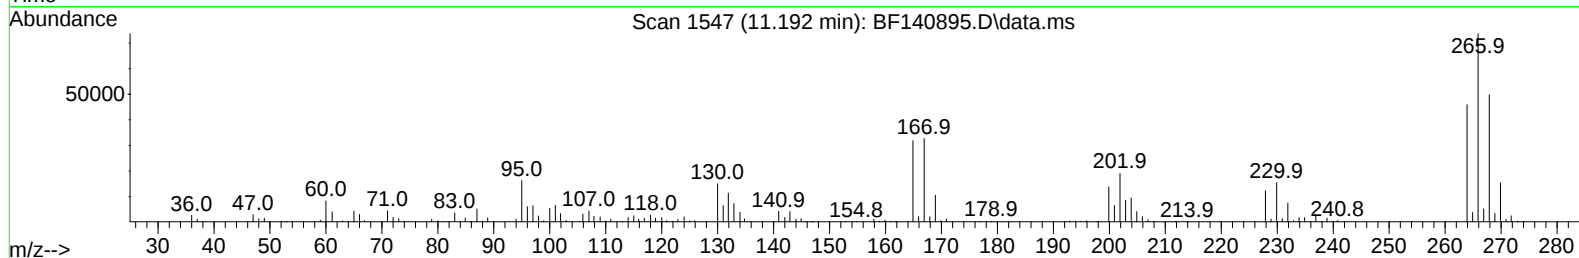


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121824\
Data File : BF140895.D
Acq On : 18 Dec 2024 09:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 18 11:45:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration

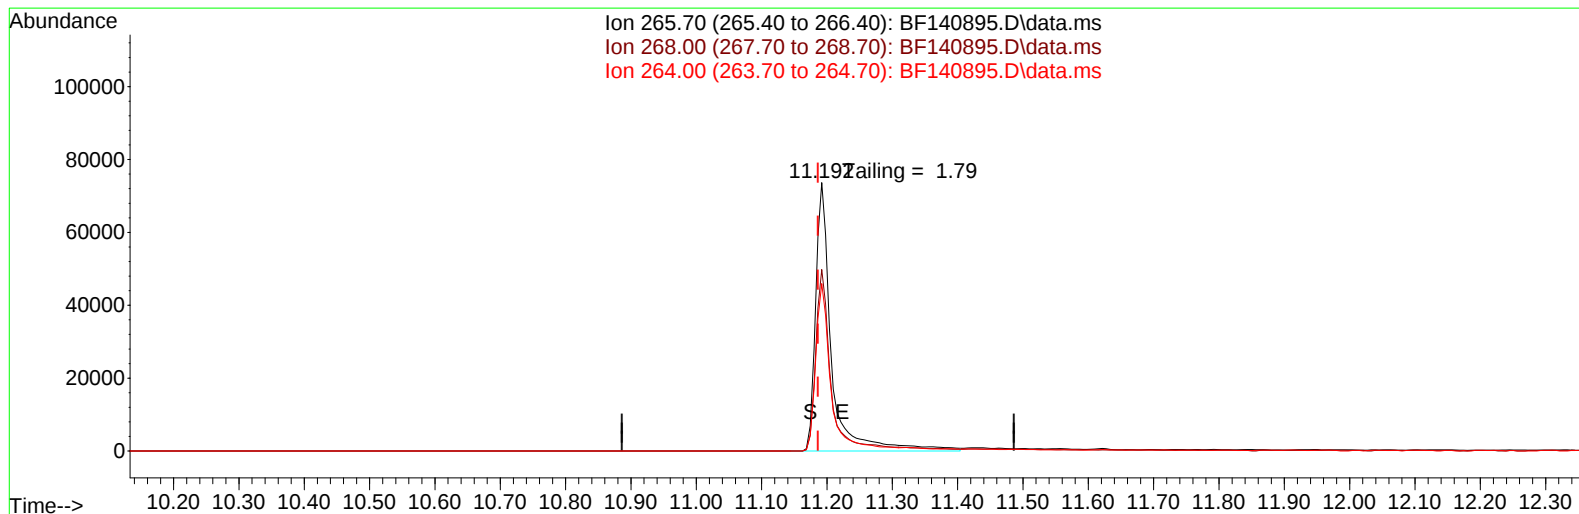

TIC: BF140895.D\data.ms

(70) Pentachlorophenol (C)




11.192min (+ 0.006) 3663.45 ng m

response 126345

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	67.63
264.00	61.80	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121824\
Data File : BF140895.D
Acq On : 18 Dec 2024 09:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 18 11:45:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration

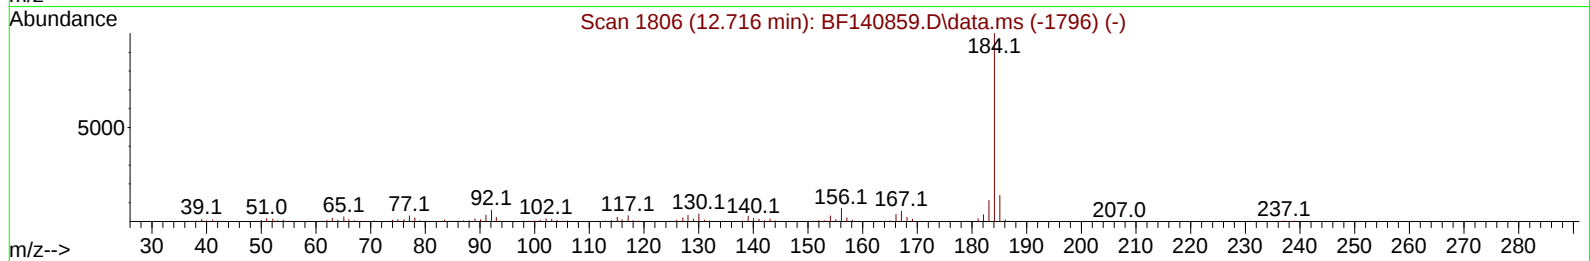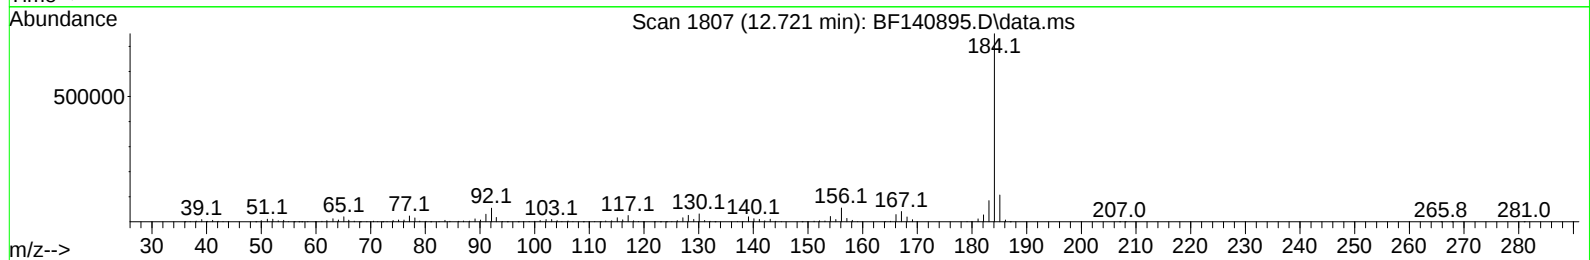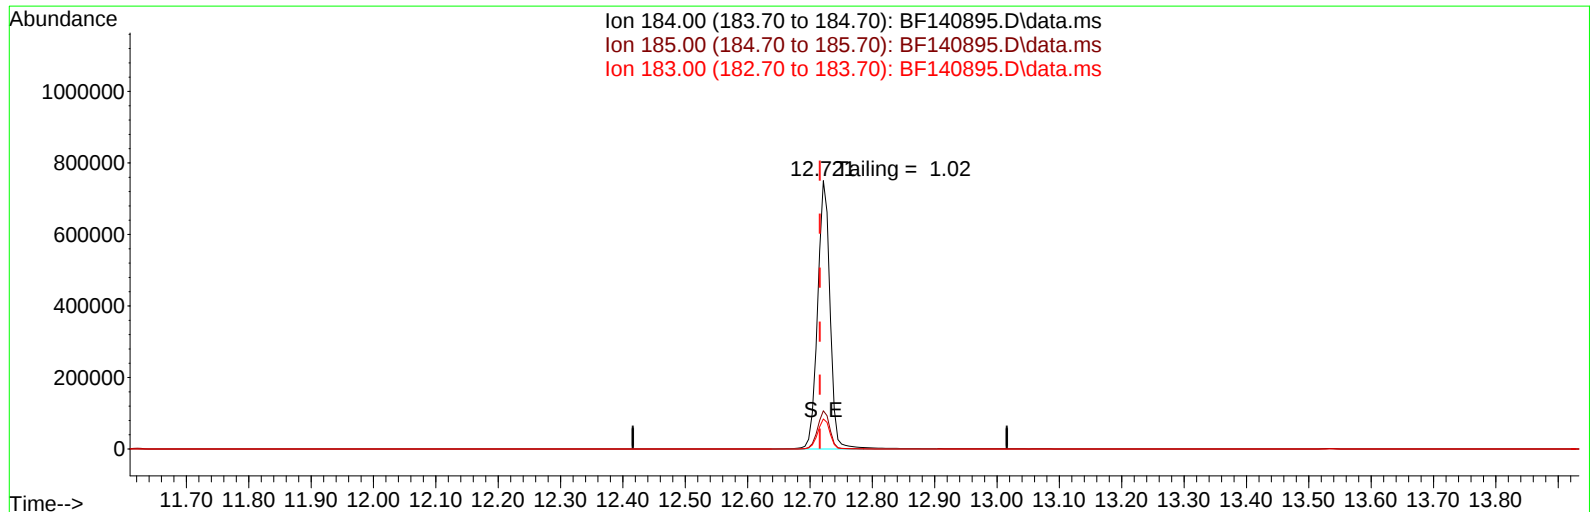

TIC: BF140895.D\data.ms

(77) Benzidine**12.721min (+ 0.005) 6539.55 ng****response 1054410**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.27
183.00	11.20	11.25
0.00	0.00	0.00