

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121824\
 Data File : BF140901.D
 Acq On : 18 Dec 2024 13:12
 Operator : RC/JU
 Sample : PB165682BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB165682BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.199	6	18	26	rVB	46353	95655	2.48%	0.528%
2	5.498	573	579	613	rBV	1408556	1950621	50.62%	10.773%
3	6.498	743	749	776	rBV	1429672	2027488	52.62%	11.198%
4	6.845	803	808	818	rVB	269215	334432	8.68%	1.847%
5	7.416	898	905	920	rBV	988683	1420329	36.86%	7.844%
6	8.128	1020	1026	1040	rBV	402400	533467	13.84%	2.946%
7	9.204	1202	1209	1214	rBV	2407098	3326332	86.32%	18.371%
8	9.880	1318	1324	1339	rVB	506375	680439	17.66%	3.758%
9	10.680	1454	1460	1490	rBV	1478700	2051282	53.23%	11.329%
10	11.374	1573	1578	1588	rBV	547580	694310	18.02%	3.835%
11	12.963	1842	1848	1853	rBV	2871806	3853375	100.00%	21.282%
12	14.027	2024	2029	2041	rBV	461187	634734	16.47%	3.506%
13	15.527	2278	2284	2298	rBV	285351	503588	13.07%	2.781%




Sum of corrected areas: 18106052

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121824\
Data File : BF140901.D
Acq On : 18 Dec 2024 13:12
Operator : RC/JU
Sample : PB165682BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165682BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

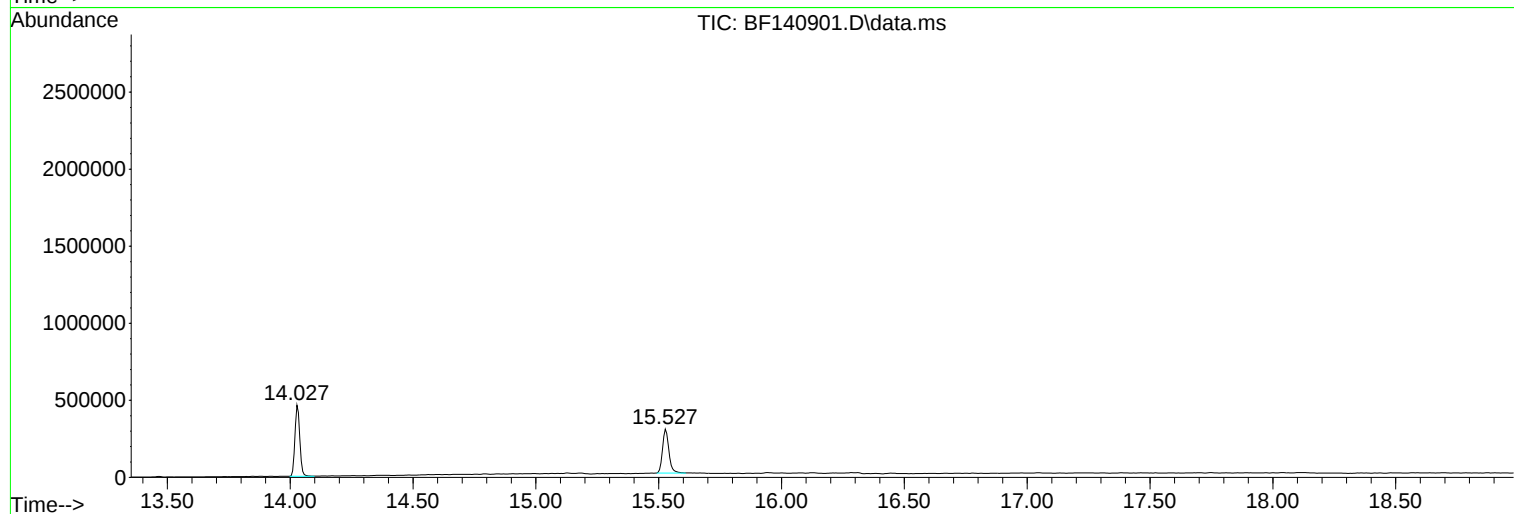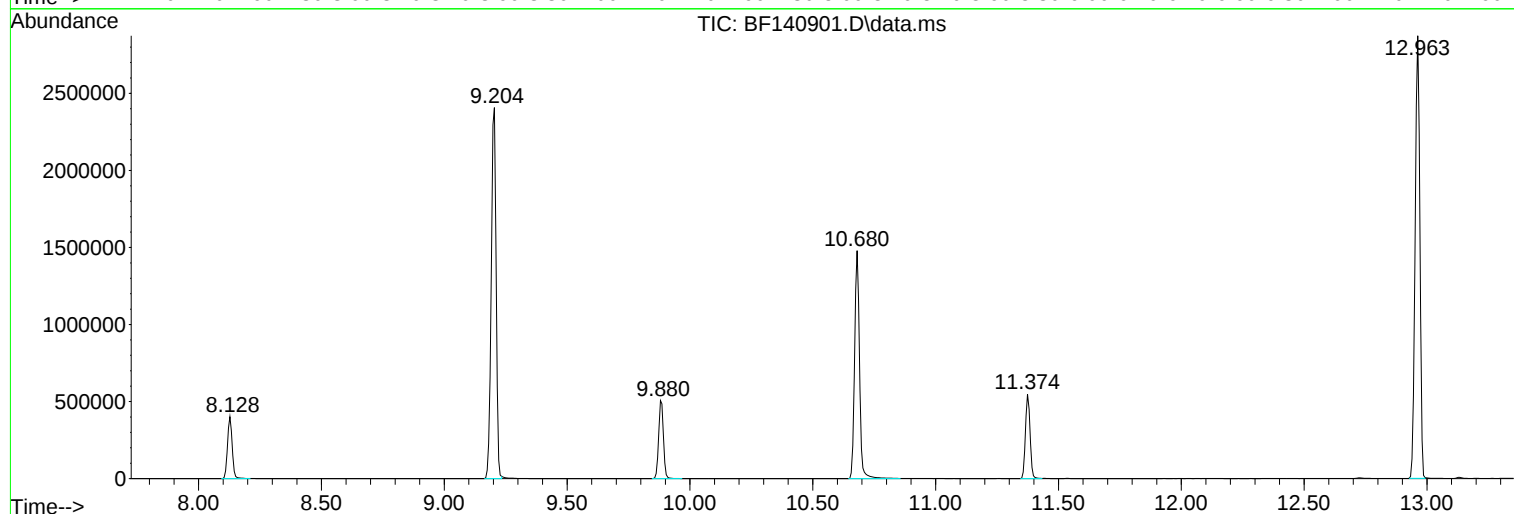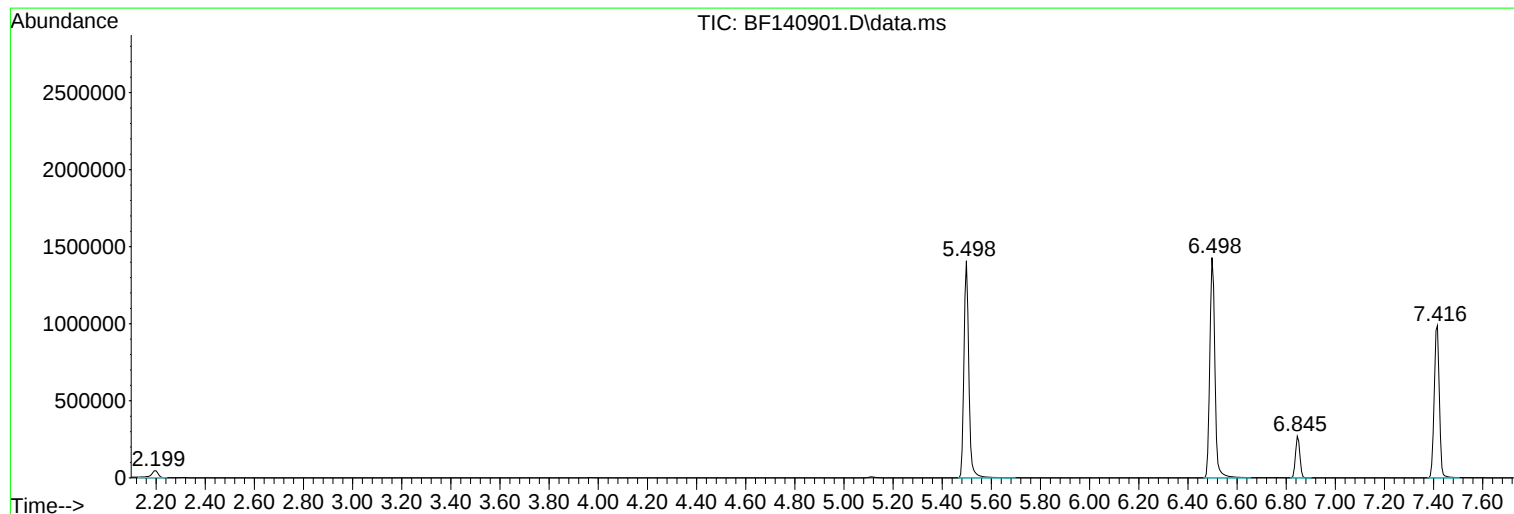

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121824\
Data File : BF140901.D
Acq On : 18 Dec 2024 13:12
Operator : RC/JU
Sample : PB165682BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165682BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.199	5.72 ng	95655	1,4-Dichlorobenzene-d4	6.845

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	90
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43
3			N-Ethylformamide	73	C3H7NO	000627-45-2	9
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
5			1,4-Butanediamine	88	C4H12N2	000110-60-1	9

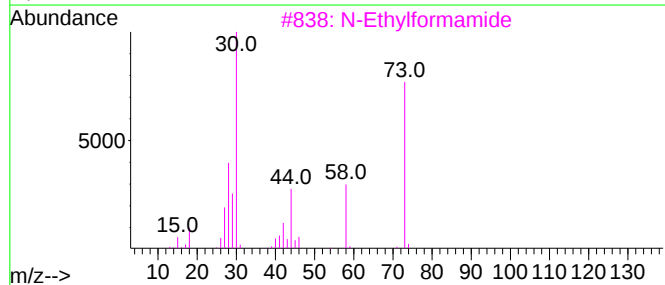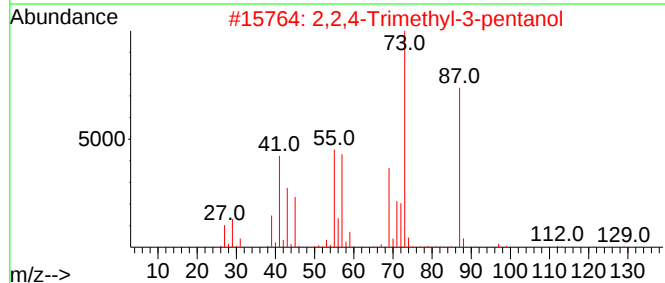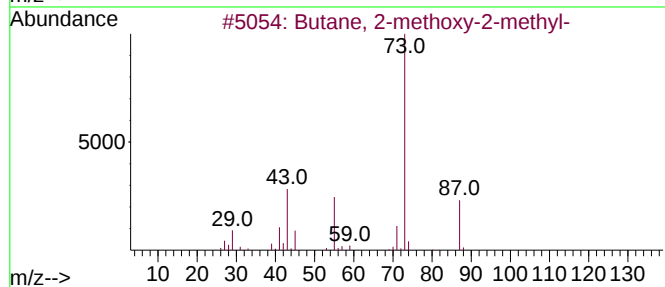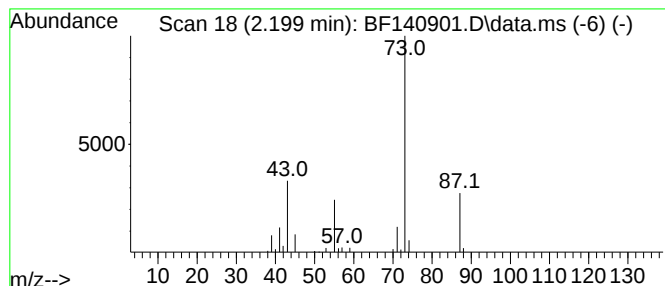

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121824\
Data File : BF140901.D
Acq On : 18 Dec 2024 13:12
Operator : RC/JU
Sample : PB165682BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165682BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.199	5.7	ng	95655	1	6.845	334432	20.0