


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121915\
 Data File : BF083934.D
 Acq On : 19 Dec 2015 1:02
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 18 14:23:22 2015

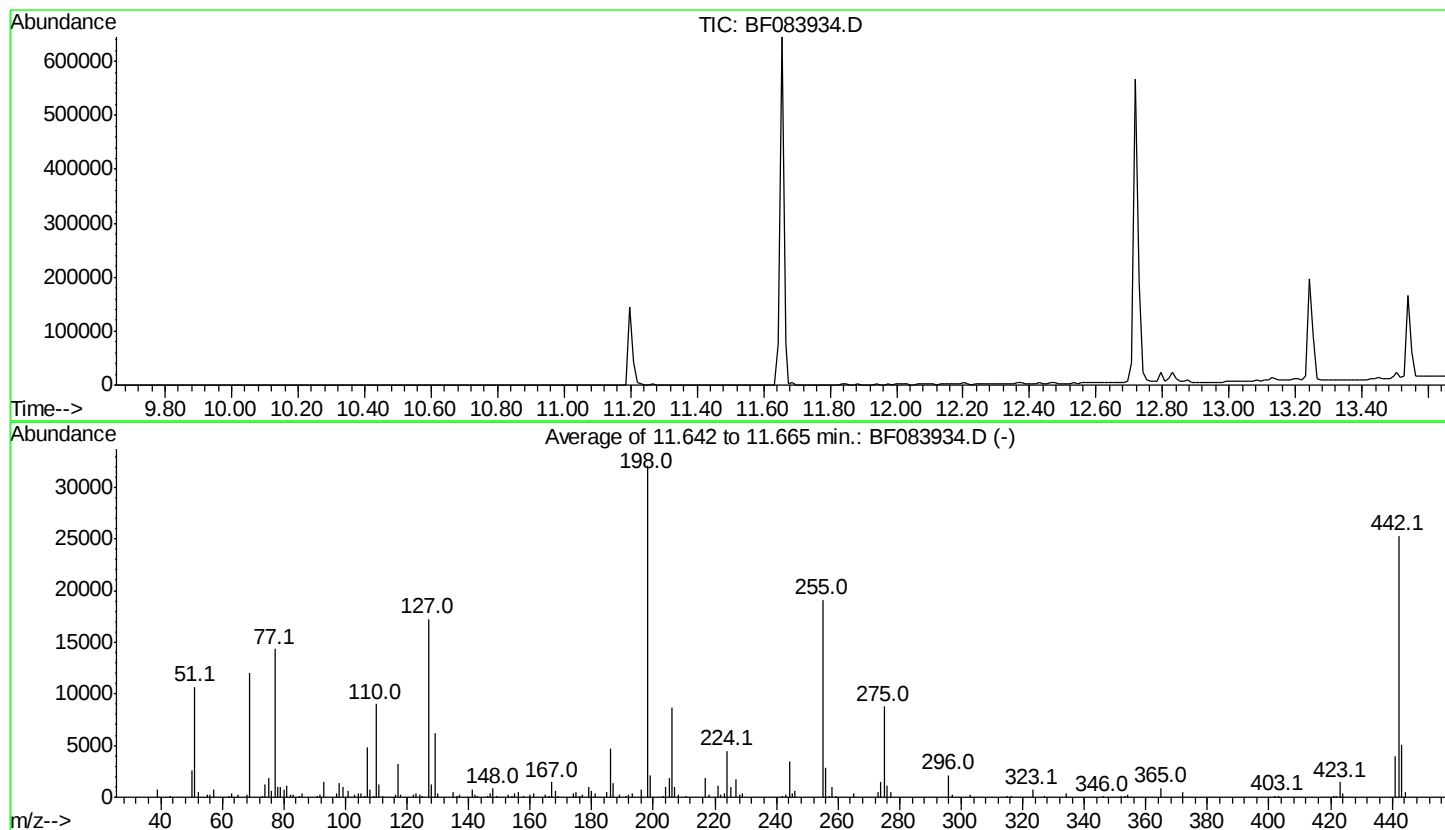

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 833

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	10704	PASS
68	69	0.00	2	1.9	226	PASS
69	198	0.00	100	37.3	11963	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.8	17267	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	32076	PASS
199	198	5	9	6.7	2146	PASS
275	198	10	60	27.4	8774	PASS
365	198	1	100	2.8	913	PASS
441	442	0.01	24	15.5	3930	PASS
442	198	50	100	78.9	25297	PASS
443	442	15	24	19.9	5045	PASS