

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121916\
 Data File : BF091796.D
 Acq On : 20 Dec 2016 1:53
 Operator : UM/SJ
 Sample : H6126-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-35

Quant Time: Dec 20 03:18:04 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 17 22:53:54 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.76	152	246117	20.00	ng	-0.01
21) Naphthalene-d8	8.04	136	957999	20.00	ng	-0.02
38) Acenaphthene-d10	9.79	164	470692	20.00	ng	-0.02
63) Phenanthrene-d10	11.28	188	795443	20.00	ng	-0.01
75) Chrysene-d12	13.91	240	602168	20.00	ng	-0.02
86) Perylene-d12	15.30	264	475675	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	1069295	72.79	ng	0.00
7) Phenol-d6	6.41	99	851101	47.51	ng	-0.01
23) Nitrobenzene-d5	7.32	82	1677868	101.00	ng	-0.02
41) 2,4,6-Tribromophenol	10.59	330	586533	146.95	ng	-0.01
44) 2-Fluorobiphenyl	9.13	172	2606070	111.23	ng	-0.01
78) Terphenyl-d14	12.87	244	2060733	86.41	ng	-0.01
Target Compounds						
9) Benzaldehyde	6.41	77	1382	Below Cal	#	1
19) n-Nitroso-di-n-propylamine	7.32	70	220972	18.54	ng	# 77
25) Isophorone	7.32	82	1445443	45.60	ng	# 65
49) Dimethylphthalate	9.52	163	99857	3.25	ng	# 99
50) 2,6-Dinitrotoluene	9.79	165	60884	9.03	ng	# 31
56) 2,4-Dinitrotoluene	9.79	165	60874	7.23	ng	# 20
66) 4-Bromophenyl-phenylether	10.59	248	37160	4.46	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121916\
Data File : BF091796.D
Acq On : 20 Dec 2016 1:53
Operator : UM/SJ
Sample : H6126-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-35

Quant Time: Dec 20 03:18:04 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 22:53:54 2016
Response via : Initial Calibration




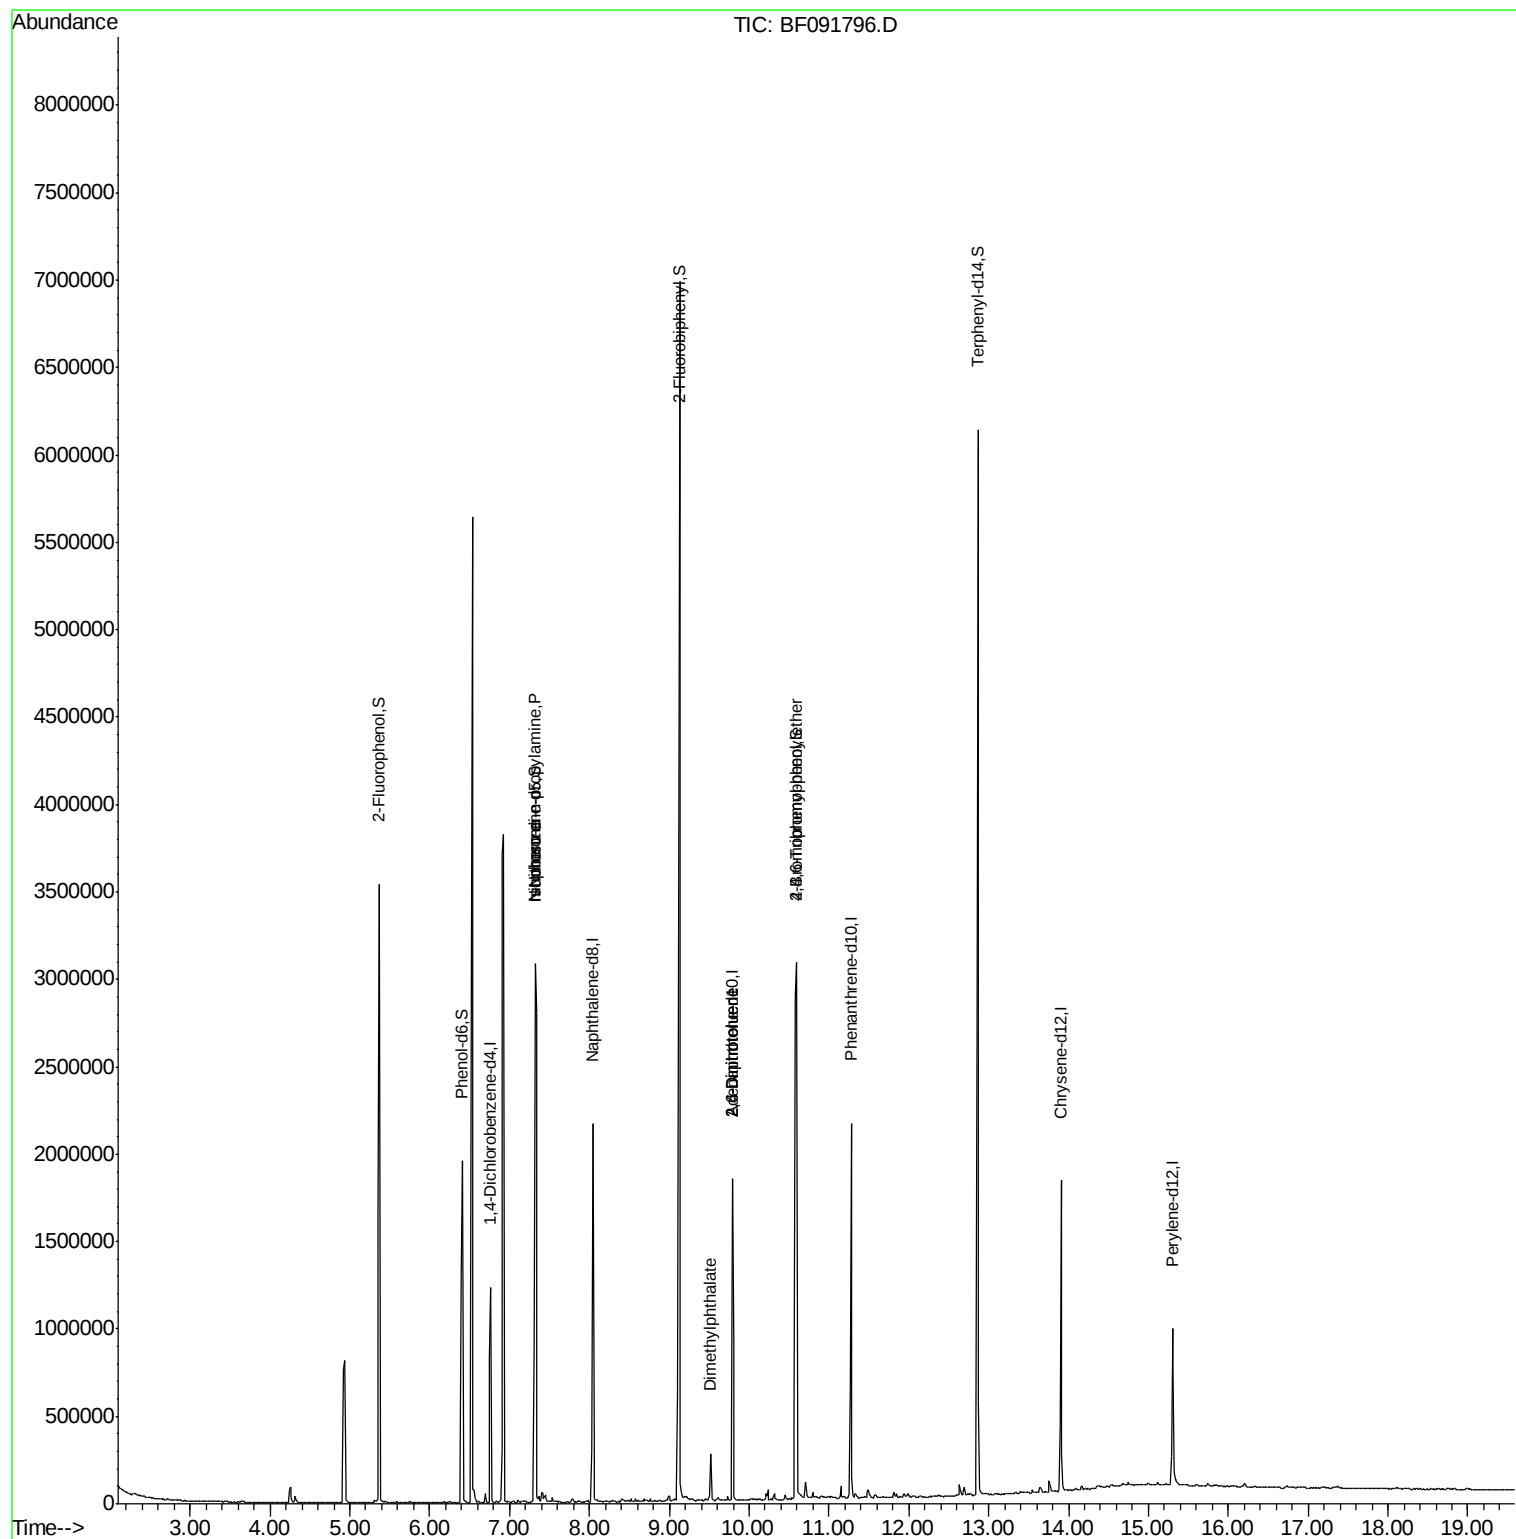


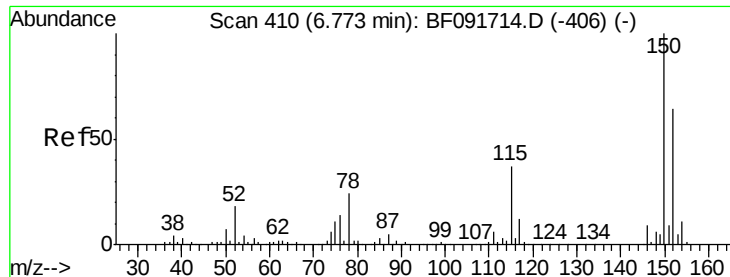

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.76 min Scan# 409
 Delta R.T. -0.01 min
 Lab File: BF091796.D
 Acq: 20 Dec 2016 1:53




Instrument :
 BNA_F
 ClientSampled :
 MW-35


Tgt Ion:152 Resp: 246117
 Ion Ratio Lower Upper
 152 100
 150 150.7 124.9 187.3
 115 52.6 46.0 69.0

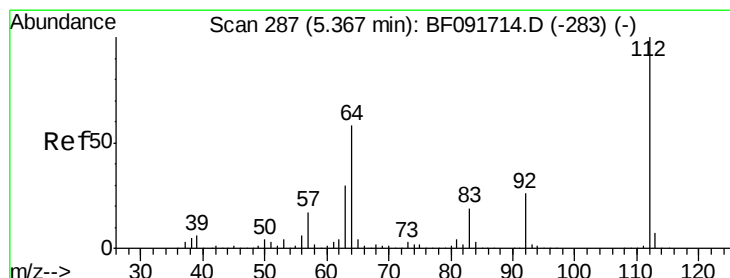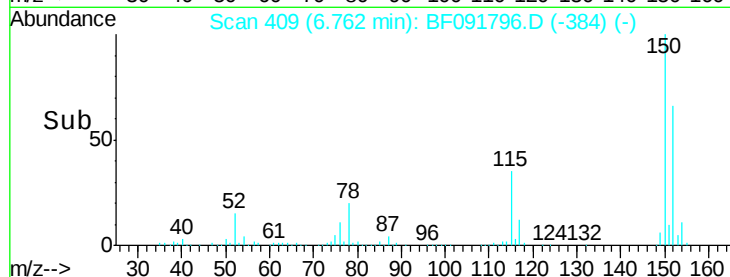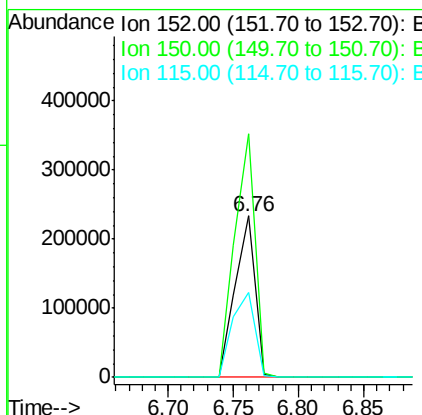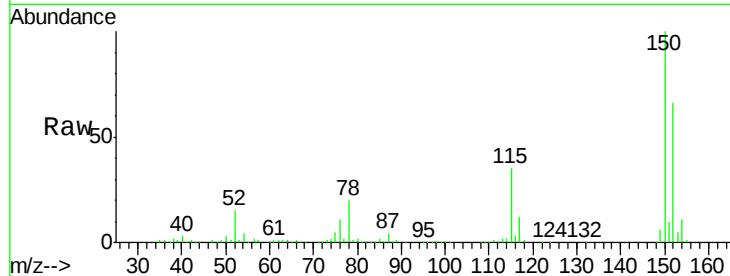

#5
 2-Fluorophenol
 Concen: 72.79 ng
 RT: 5.37 min Scan# 287
 Delta R.T. 0.00 min
 Lab File: BF091796.D
 Acq: 20 Dec 2016 1:53

Tgt Ion:112 Resp: 1069295
 Ion Ratio Lower Upper
 112 100
 64 56.6 46.1 69.1
 63 29.2 23.8 35.6

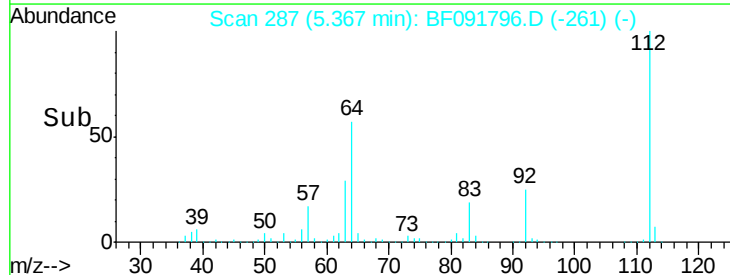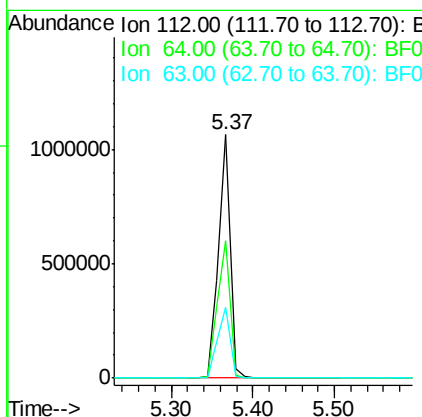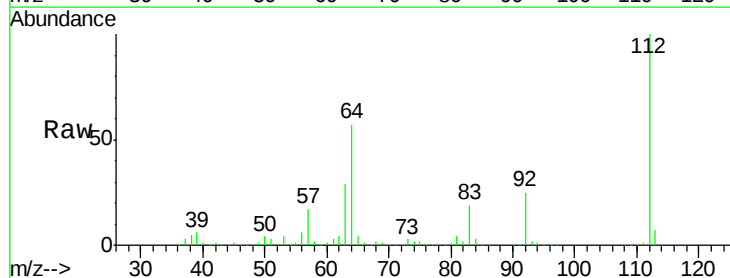

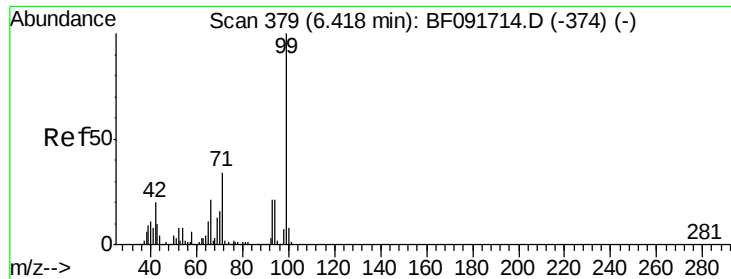

#7

Phenol-d6

Concen: 47.51 ng

RT: 6.41 min Scan# 378

Delta R.T. -0.01 min

Lab File: BF091796.D

Acq: 20 Dec 2016 1:53

Instrument :

BNA_F

ClientSampleId :

MW-35





Tgt Ion: 99 Resp: 851101

Ion Ratio Lower Upper

99 100

42 14.1 15.6 23.4#

71 29.5 27.5 41.3

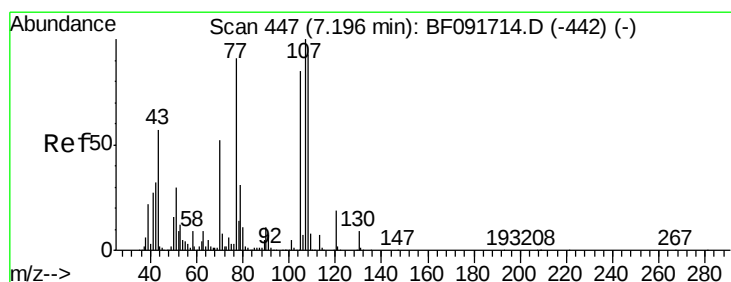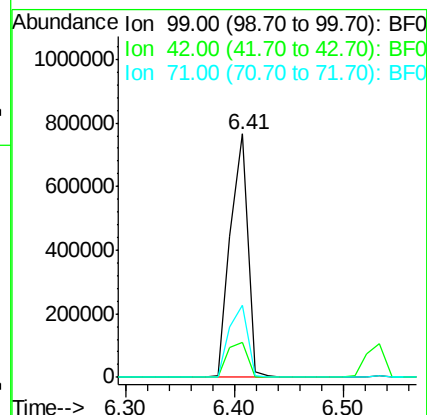

#19

n-Nitroso-di-n-propylamine

Concen: 18.54 ng

RT: 7.32 min Scan# 458

Delta R.T. 0.13 min

Lab File: BF091796.D

Acq: 20 Dec 2016 1:53

Tgt Ion: 70 Resp: 220972




Ion Ratio Lower Upper


70 100

42 47.6 49.4 74.0#

101 0.0 7.4 11.2#

130 1.9 14.2 21.4#

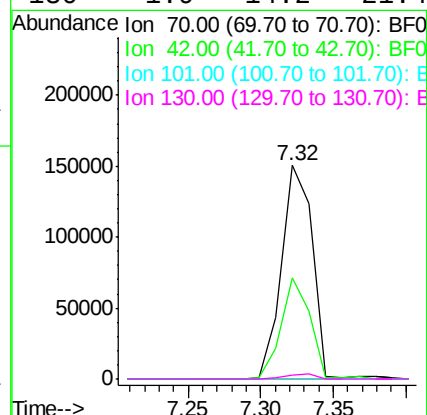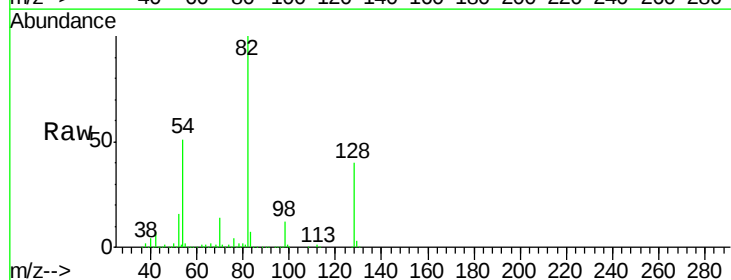

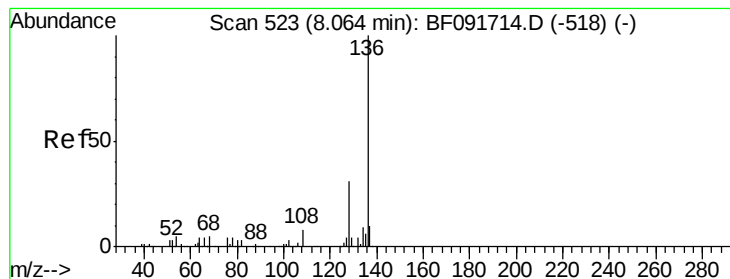

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.04 min Scan# 521

Delta R.T. -0.02 min

Lab File: BF091796.D

Acq: 20 Dec 2016 1:53

Instrument :

BNA_F

ClientSampleId :

MW-35

Tgt Ion: 136 Resp: 957999


Ion Ratio Lower Upper

136 100

137 11.2 8.4 12.6

54 8.3 4.5 6.7#

68 6.8 3.6 5.4#



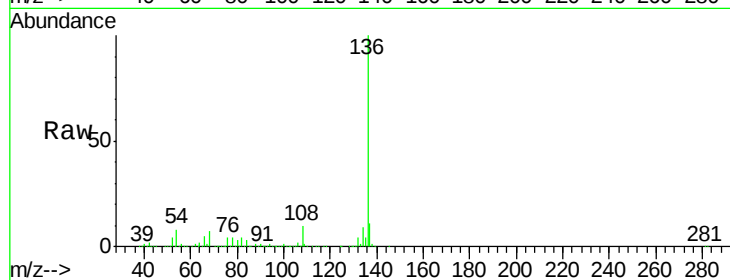


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

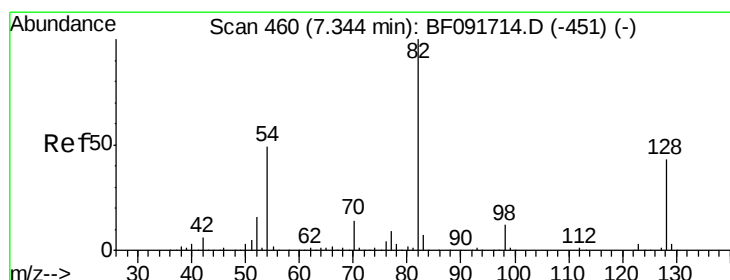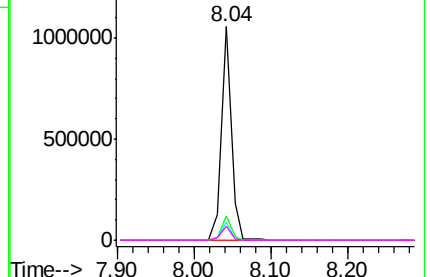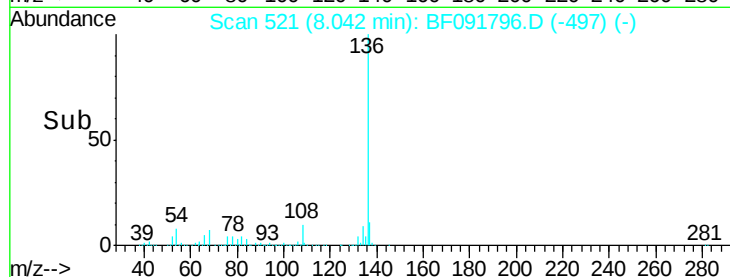

#23

Nitrobenzene-d5

Concen: 101.00 ng

RT: 7.32 min Scan# 458

Delta R.T. -0.02 min

Lab File: BF091796.D

Acq: 20 Dec 2016 1:53


Tgt Ion: 82 Resp: 1677868

Ion Ratio Lower Upper

82 100

128 40.2 34.6 52.0



54 51.2 39.5 59.3

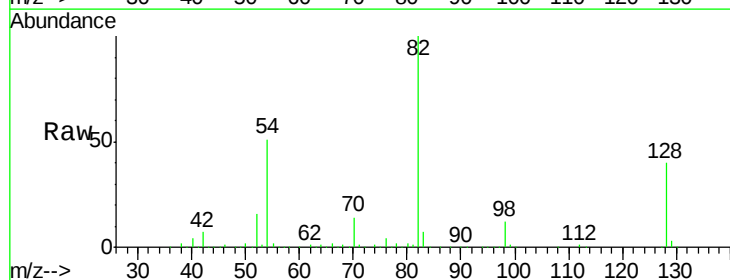


Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

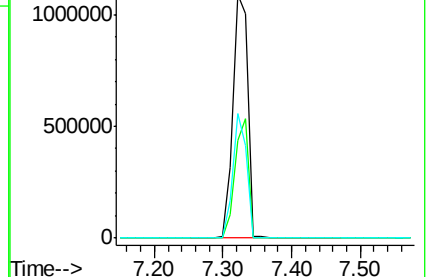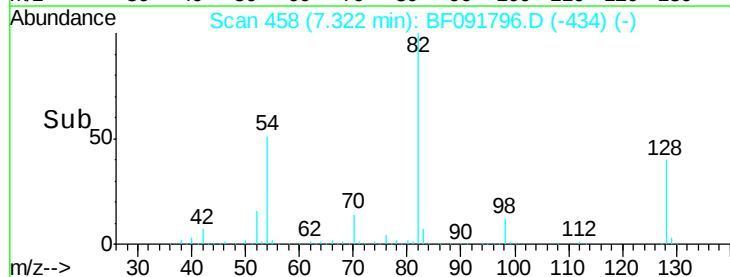



#25

Isophorone

Concen: 45.60 ng

RT: 7.32 min Scan# 458

Delta R.T. -0.29 min

Lab File: BF091796.D

Acq: 20 Dec 2016 1:53

Instrument :

BNA_F

ClientSampleId :

MW-35





Tgt Ion: 82 Resp: 1445443

Ion Ratio Lower Upper

82 100

95 0.0 5.6 8.4#

138 0.0 14.6 22.0#

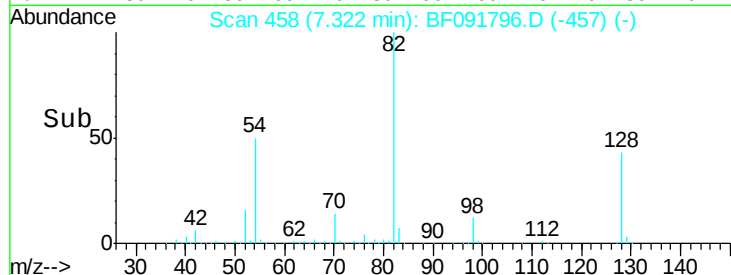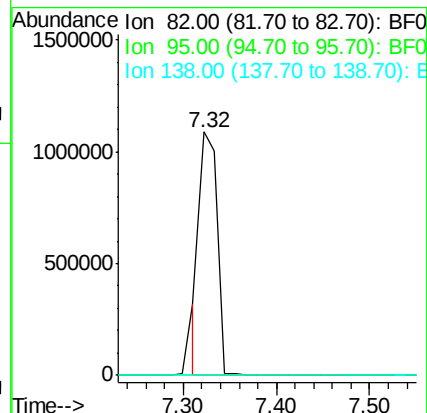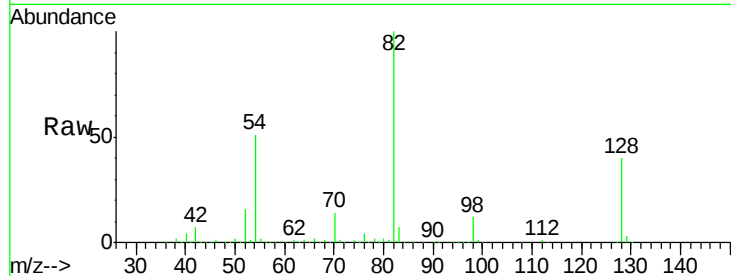

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.79 min Scan# 674

Delta R.T. -0.02 min

Lab File: BF091796.D

Acq: 20 Dec 2016 1:53




Tgt Ion: 164 Resp: 470692


Ion Ratio Lower Upper

164 100

162 103.1 80.2 120.2

160 45.4 36.9 55.3

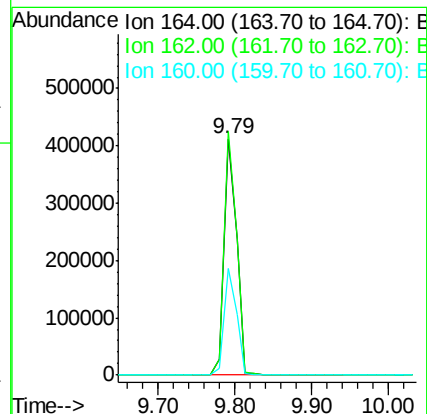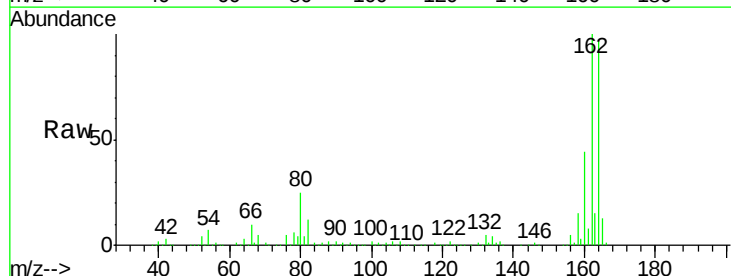







#41
 2,4,6-Tribromophenol
 Concen: 146.95 ng
 RT: 10.59 min Scan# 744
 Delta R.T. -0.01 min
 Lab File: BF091796.D
 Acq: 20 Dec 2016 1:53

Instrument :
 BNA_F
 ClientSampleId :
 MW-35

Tgt Ion:330 Resp: 586533
 Ion Ratio Lower Upper
 330 100
 332 95.3 77.4 116.2
 141 34.5 34.1 51.1

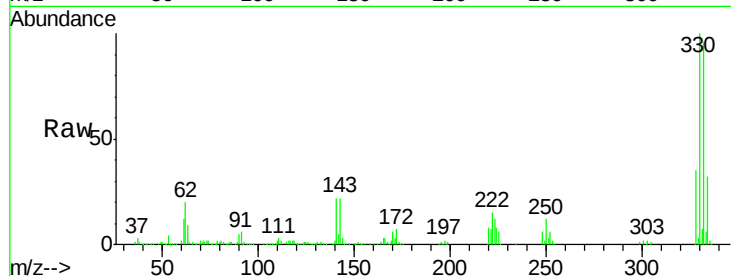


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


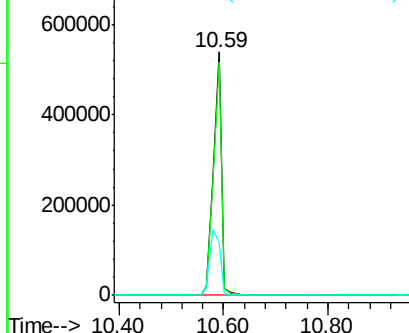



#44
 2-Fluorobiphenyl
 Concen: 111.23 ng
 RT: 9.13 min Scan# 616
 Delta R.T. -0.01 min
 Lab File: BF091796.D
 Acq: 20 Dec 2016 1:53

Tgt Ion:172 Resp: 2606070
 Ion Ratio Lower Upper
 172 100
 171 36.3 29.4 44.0
 170 25.1 20.2 30.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

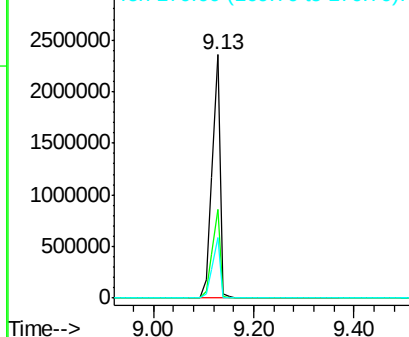

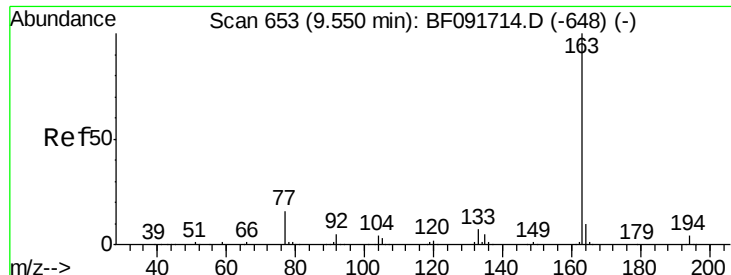

#49

Dimethylphthalate

Concen: 3.25 ng

RT: 9.52 min Scan# 650

Delta R.T. -0.03 min

Lab File: BF091796.D

Acq: 20 Dec 2016 1:53

Instrument :

BNA_F

ClientSampleId :

MW-35


Tgt Ion:163 Resp: 99857

Ion Ratio Lower Upper

163 100

194 2.9 3.0 4.4#




164 10.3 8.0 12.0



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

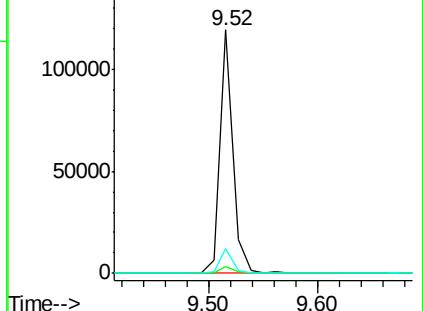

#50

2,6-Dinitrotoluene

Concen: 9.03 ng

RT: 9.79 min Scan# 674

Delta R.T. 0.18 min

Lab File: BF091796.D

Acq: 20 Dec 2016 1:53


Tgt Ion:165 Resp: 60884

Ion Ratio Lower Upper

165 100

63 1.4 36.2 54.4#



89 1.2 40.2 60.4#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0



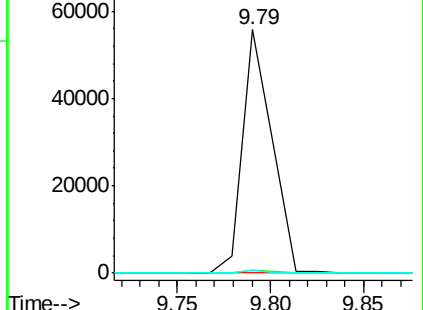



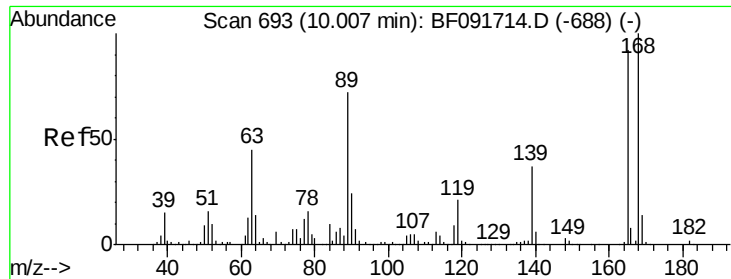

#56
 2,4-Dinitrotoluene
 Concen: 7.23 ng
 RT: 9.79 min Scan# 674
 Delta R.T. -0.22 min
 Lab File: BF091796.D
 Acq: 20 Dec 2016 1:53




Instrument :
 BNA_F
 ClientSampleId :
 MW-35


Tgt Ion:	165	Resp:	60874
Ion	Ratio	Lower	Upper
165	100		
63	1.4	40.2	60.4#
89	1.2	62.5	93.7#
182	0.0	1.8	2.8#

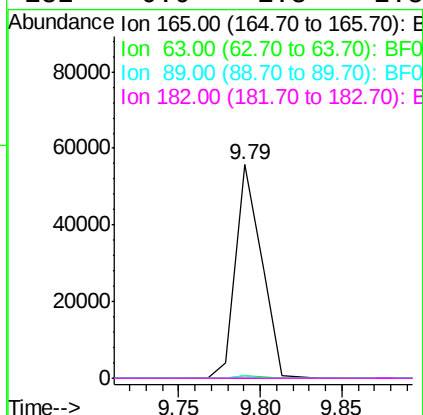

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.28 min Scan# 804
 Delta R.T. -0.01 min
 Lab File: BF091796.D
 Acq: 20 Dec 2016 1:53

Tgt Ion:	188	Resp:	795443
Ion	Ratio	Lower	Upper
188	100		
94	9.0	10.0	15.0#
80	9.4	11.2	16.8#

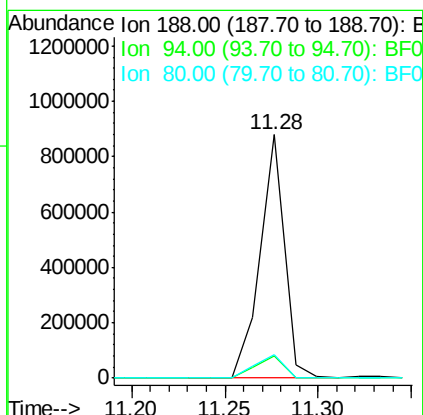

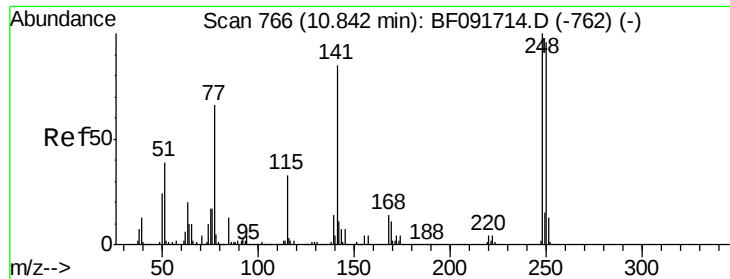

#66

4-Bromophenyl-phenylether

Concen: 4.46 ng

RT: 10.59 min Scan# 744

Delta R.T. -0.25 min

Lab File: BF091796.D

Acq: 20 Dec 2016 1:53

Instrument :

BNA_F

ClientSampleId :

MW-35


Tgt Ion:248 Resp: 37160

Ion Ratio Lower Upper

248 100

250 204.6 76.9 115.3#




141 389.3 68.2 102.4#

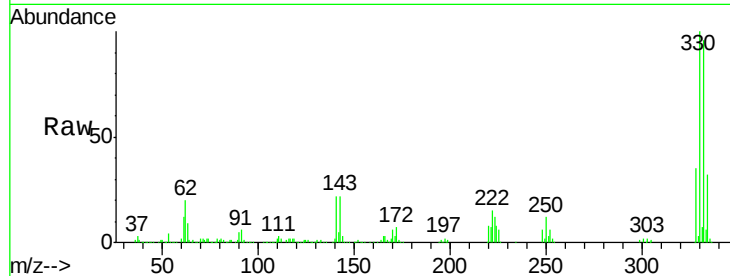

Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

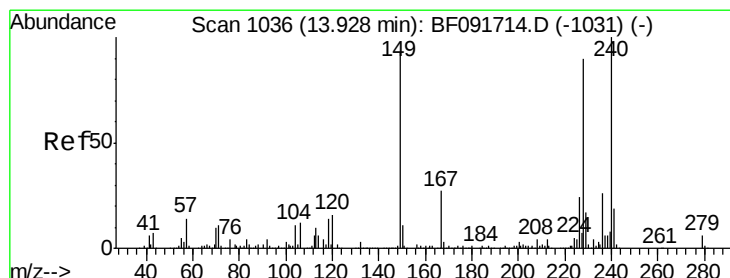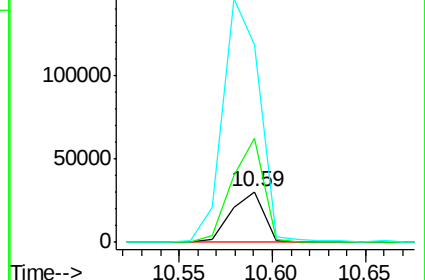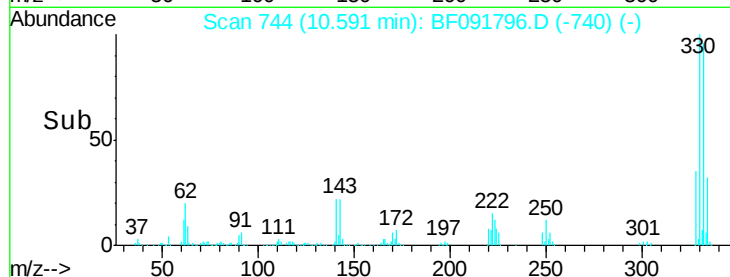

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.91 min Scan# 1034

Delta R.T. -0.02 min

Lab File: BF091796.D

Acq: 20 Dec 2016 1:53


Tgt Ion:240 Resp: 602168

Ion Ratio Lower Upper

240 100

120 11.7 12.9 19.3#



236 25.5 20.9 31.3

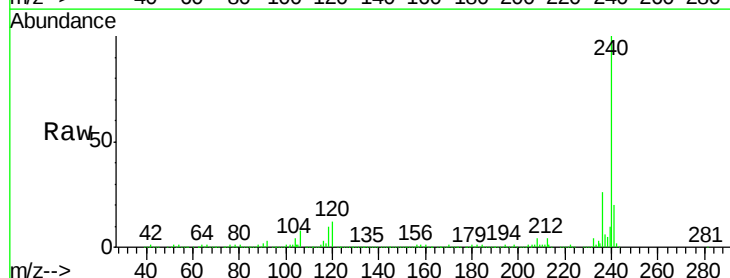


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

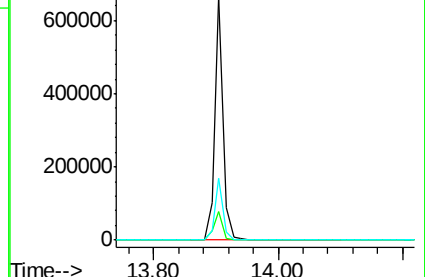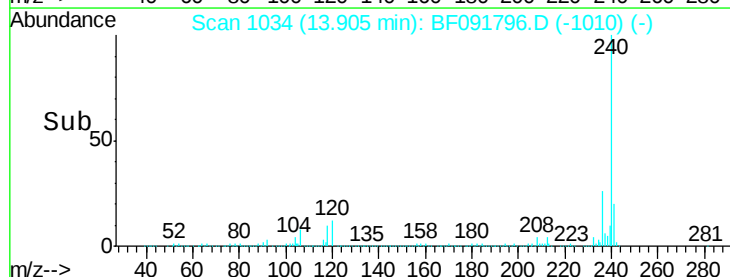







#78
 Terphenyl-d14
 Concen: 86.41 ng
 RT: 12.87 min Scan# 943
 Delta R.T. -0.01 min
 Lab File: BF091796.D
 Acq: 20 Dec 2016 1:53

Instrument :
 BNA_F
 ClientSampleId :
 MW-35

Tgt Ion:244 Resp: 2060733
 Ion Ratio Lower Upper
 244 100
 212 7.6 6.2 9.2
 122 13.5 11.4 17.2

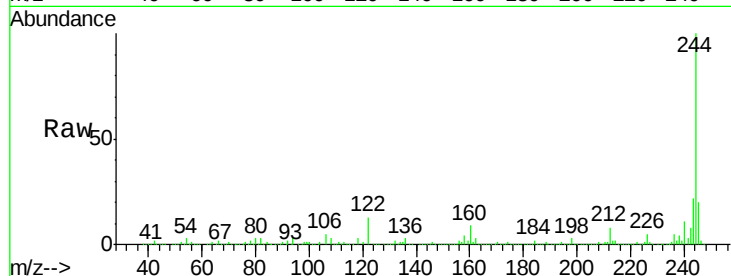


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

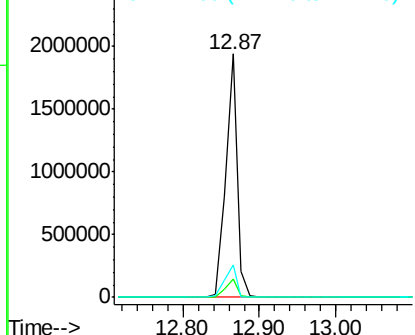

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.30 min Scan# 1156
 Delta R.T. -0.03 min
 Lab File: BF091796.D
 Acq: 20 Dec 2016 1:53

Tgt Ion:264 Resp: 475675
 Ion Ratio Lower Upper
 264 100
 260 23.3 19.2 28.8
 265 22.3 17.4 26.0



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

