
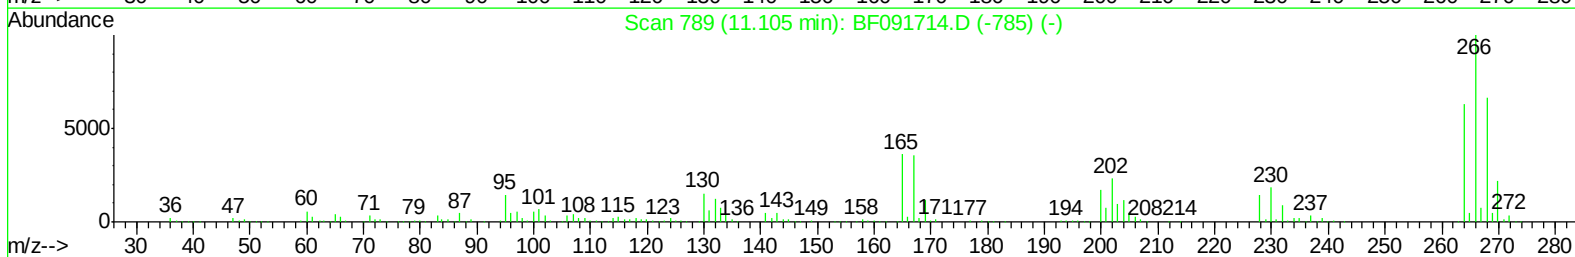
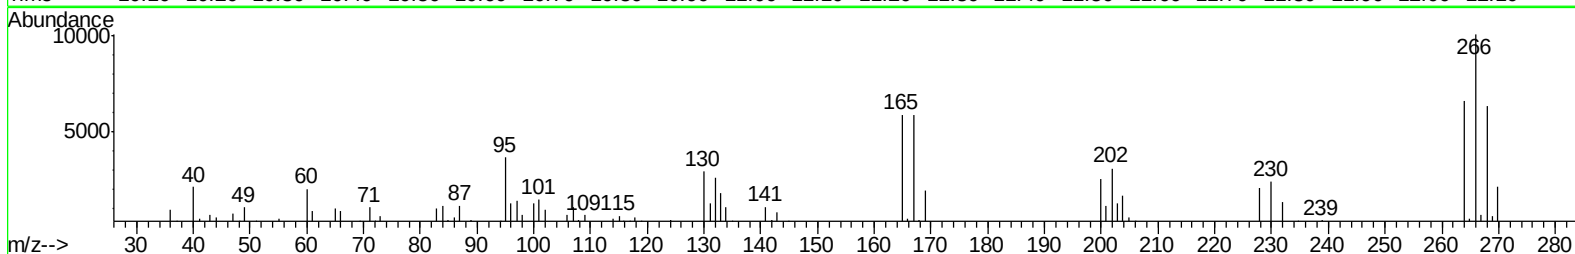


Data Path : Z:\HPCHEM1\BNA_F\Data\BF121916\
Data File : BF091778.D
Acq On : 19 Dec 2016 14:10
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 08:09:57 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 22:53:54 2016
Response via : Initial Calibration

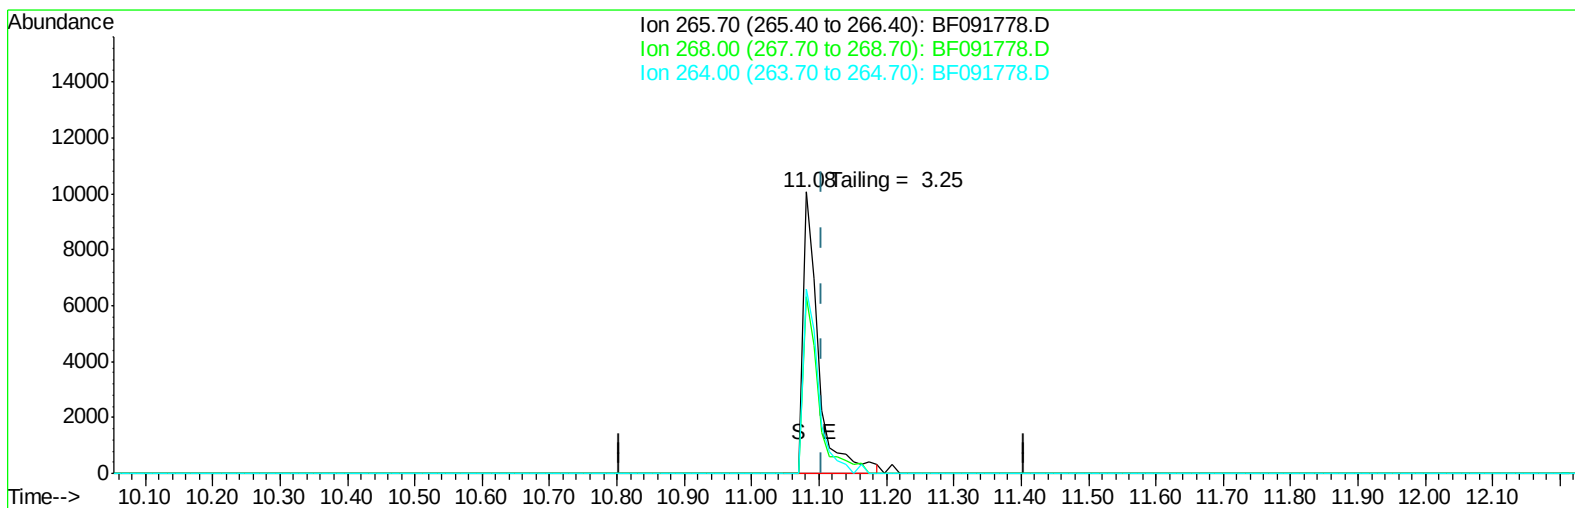

TIC: BF091778.D

(69) Pentachlorophenol (C)




11.082min (-0.023) 2913.28ng

response 16082

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	62.71
264.00	62.90	65.54
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF121916\
 Data File : BF091778.D
 Acq On : 19 Dec 2016 14:10
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 08:09:57 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 17 22:53:54 2016
 Response via : Initial Calibration

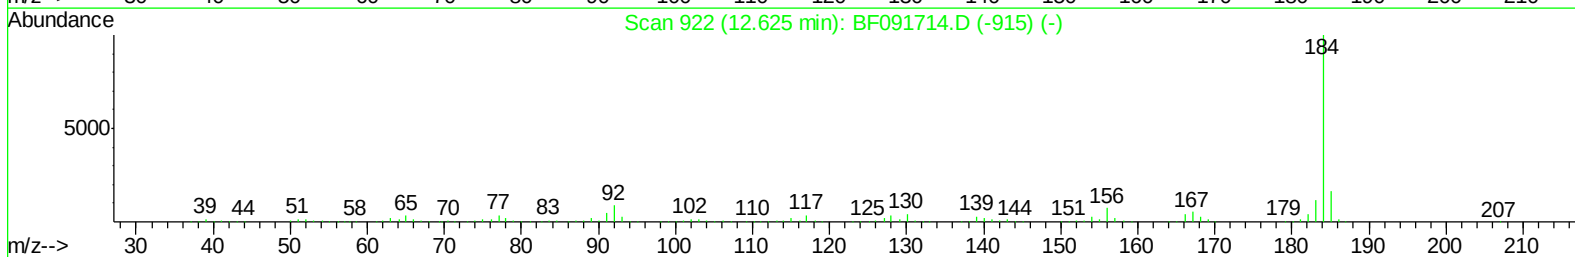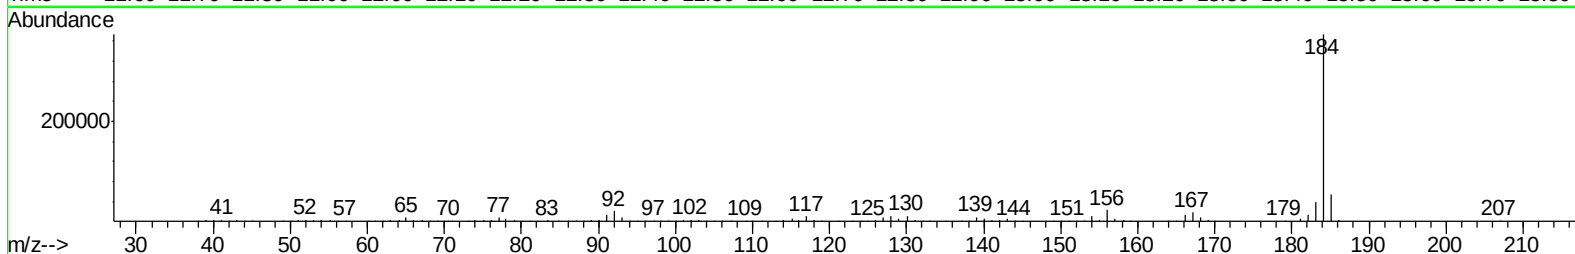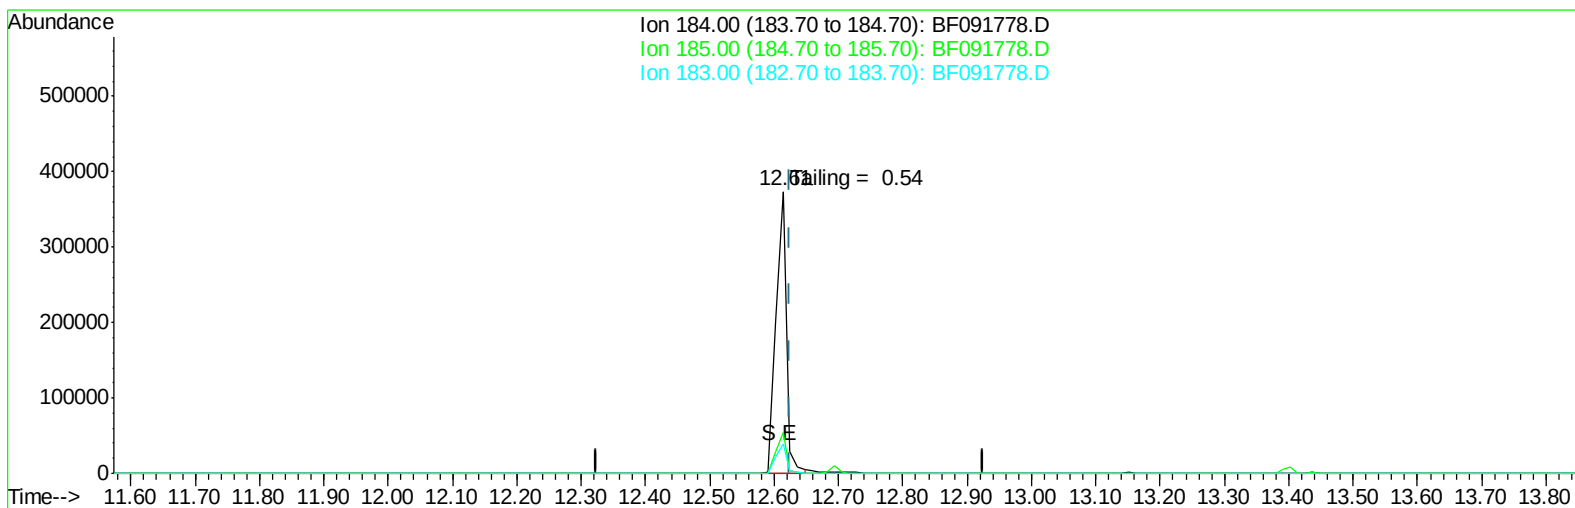

TIC: BF091778.D

(76) Benzidine

12.614min (-0.011) 15318.76ng

response 436986

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.34
183.00	11.50	10.64
0.00	0.00	0.00