
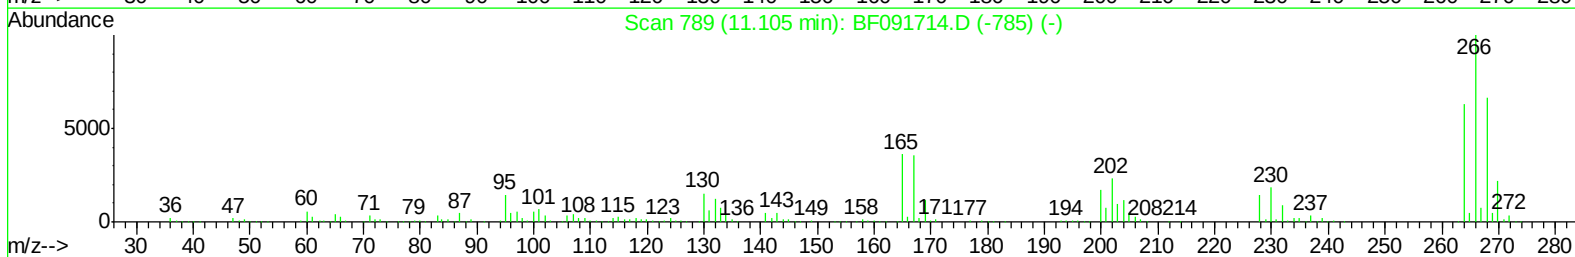
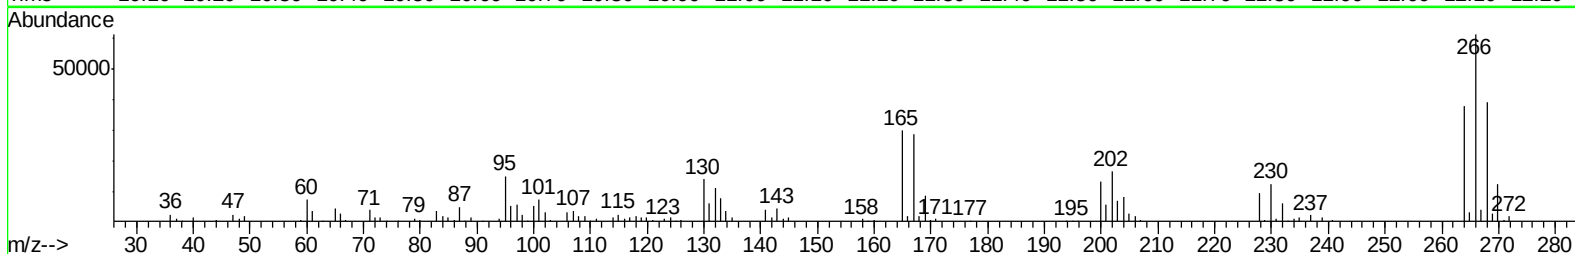


Data Path : Z:\HPCHEM1\BNA_F\Data\BF121916\
Data File : BF091781.D
Acq On : 19 Dec 2016 19:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 08:11:04 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 22:53:54 2016
Response via : Initial Calibration

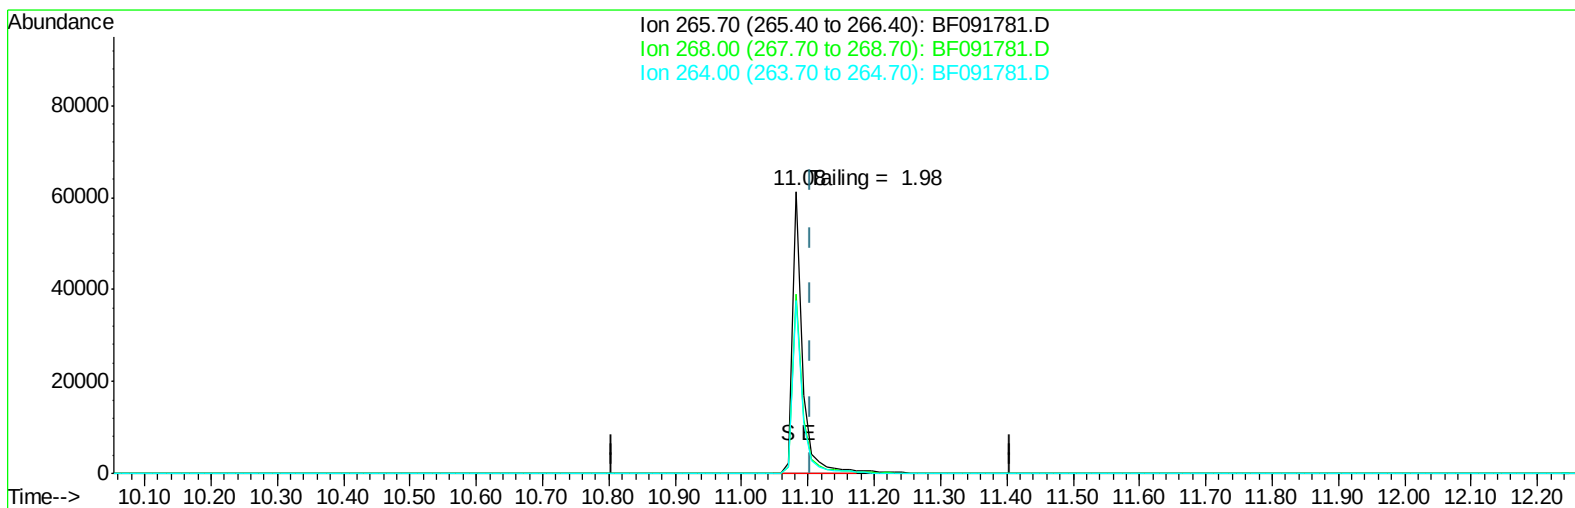

TIC: BF091781.D

(69) Pentachlorophenol (C)




11.082min (-0.022) 7924.22ng

response 64934

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	63.75
264.00	62.90	61.53
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF121916\
Data File : BF091781.D
Acq On : 19 Dec 2016 19:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 08:11:04 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 22:53:54 2016
Response via : Initial Calibration

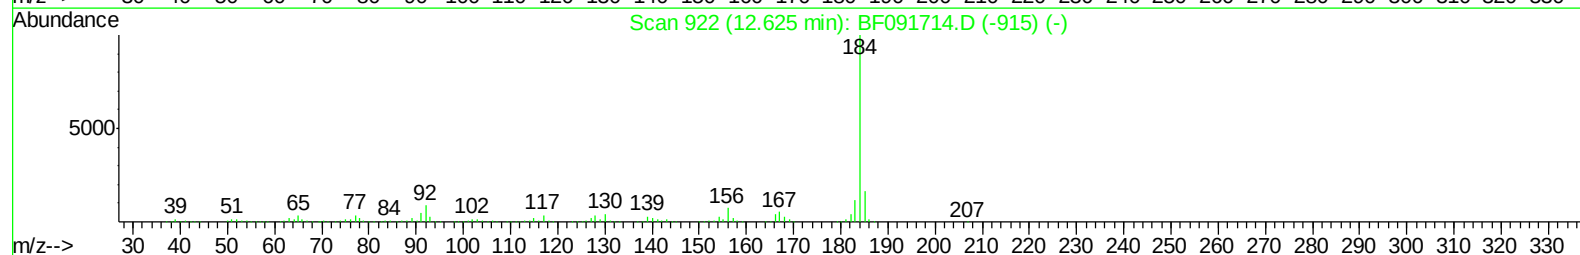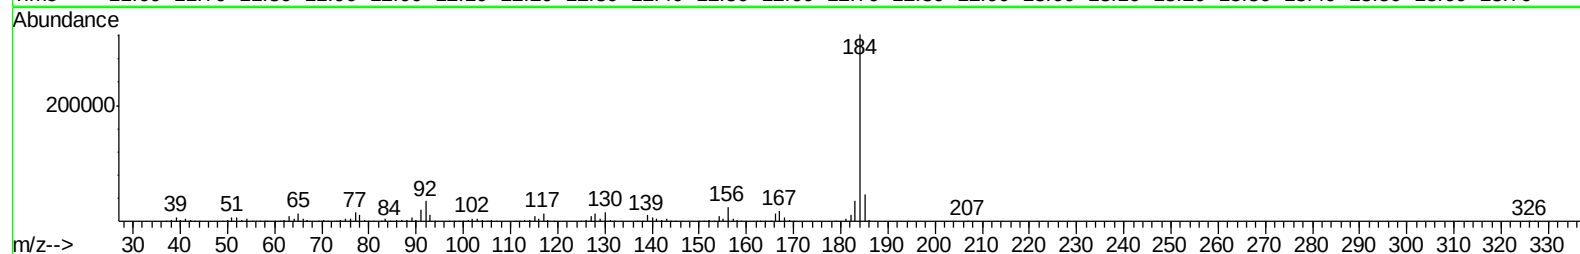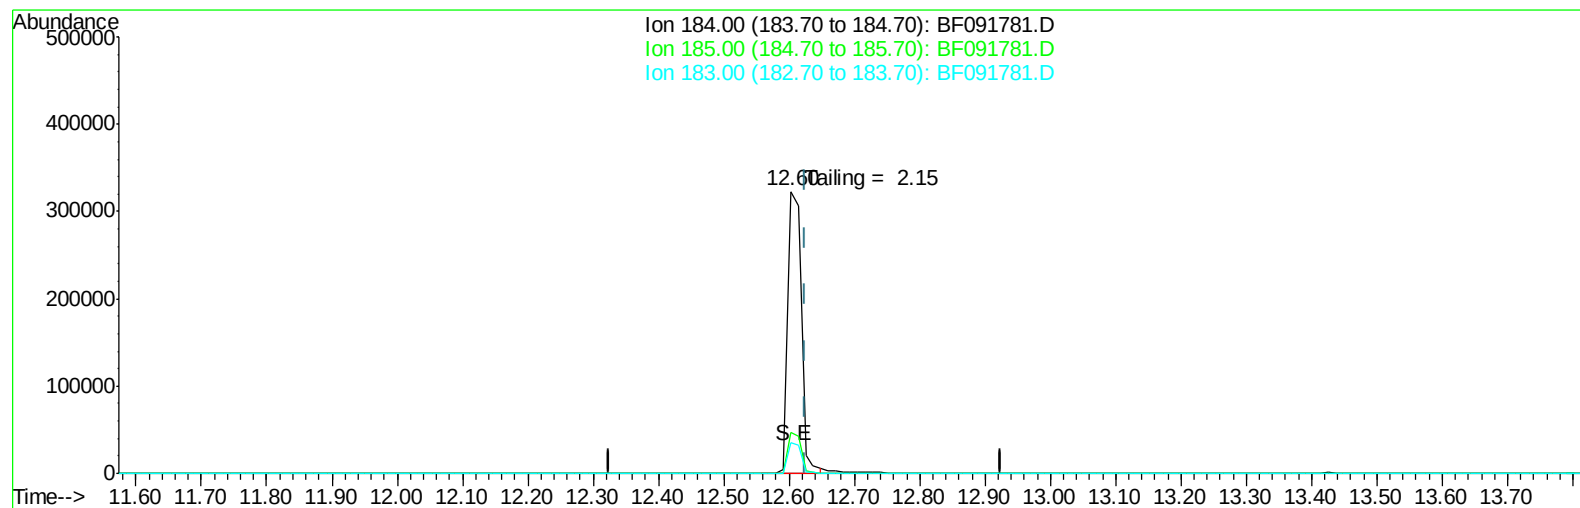

TIC: BF091781.D

(76) Benzidine

12.602min (-0.022) 6852.87ng

response 470272

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.59
183.00	11.50	10.90
0.00	0.00	0.00