

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121916\
 Data File : BF091803.D
 Acq On : 20 Dec 2016 5:06
 Operator : UM/SJ
 Sample : H6125-03RE
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-47(8-9.5)-12-14-16RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.635	39	48	51	rVV	241271	584138	2.50%	0.114%
2	2.978	69	78	84	rVB2	106993	378248	1.62%	0.074%
3	3.161	84	94	99	rBV3	133690	370905	1.59%	0.072%
4	3.436	112	118	125	rVB	246033	683964	2.92%	0.133%
5	3.664	135	138	142	rVB	144262	282852	1.21%	0.055%
6	3.767	142	147	150	rBV	325193	640438	2.74%	0.125%
7	3.927	154	161	163	rBV	1164615	2299395	9.83%	0.449%
8	3.973	163	165	169	rVB	553392	870706	3.72%	0.170%
9	4.087	170	175	178	rBV2	442271	932301	3.98%	0.182%
10	4.156	178	181	184	rVB	494890	935441	4.00%	0.182%
11	4.236	184	188	190	rBV	452378	656083	2.80%	0.128%
12	4.304	190	194	199	rVB2	1285835	2296858	9.82%	0.448%
13	4.407	199	203	207	rBV	718652	1231106	5.26%	0.240%
14	4.487	207	210	211	rBV	164527	250465	1.07%	0.049%
15	4.521	211	213	216	rVB2	292108	435237	1.86%	0.085%
16	4.590	216	219	221	rBV2	500283	766999	3.28%	0.150%
17	4.636	221	223	225	rBV	711277	1110189	4.74%	0.217%
18	4.681	225	227	229	rVB2	292598	418550	1.79%	0.082%
19	4.761	229	234	236	rBV	2469030	3888110	16.62%	0.758%
20	4.853	239	242	245	rVB2	3864835	5990893	25.60%	1.169%
21	4.921	245	248	250	rBV2	5011990	7121820	30.43%	1.389%
22	4.967	250	252	253	rVB2	250886	278813	1.19%	0.054%
23	5.059	256	260	264	rVB2	827947	1470726	6.29%	0.287%
24	5.139	264	267	268	rBV	4200652	6249033	26.70%	1.219%
25	5.161	268	269	276	rVB3	1383865	3180994	13.59%	0.621%
26	5.264	276	278	279	rBV	379648	525563	2.25%	0.103%
27	5.310	279	282	284	rBV2	1092446	1597108	6.83%	0.312%
28	5.367	284	287	289	rVB	3803794	4440941	18.98%	0.866%
29	5.424	289	292	295	rBV3	1691931	2618335	11.19%	0.511%
30	5.470	295	296	297	rBV	374055	325027	1.39%	0.063%
31	5.516	297	300	302	rBV	3565000	6210902	26.54%	1.212%
32	5.561	302	304	305	rVB	3852802	3966661	16.95%	0.774%
33	5.596	305	307	312	rVB2	3390994	7456908	31.87%	1.455%
34	5.676	312	314	318	rVB	1136568	1607033	6.87%	0.313%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121916\
 Data File : BF091803.D
 Acq On : 20 Dec 2016 5:06
 Operator : UM/SJ
 Sample : H6125-03RE
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-47(8-9.5)-12-14-16RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	5.767	318	322	325	rBV2	4834536	10791687	46.12%	2.105%
36	5.824	325	327	332	rVB4	1572591	3659580	15.64%	0.714%
37	5.916	332	335	338	rBV2	6071453	11377561	48.62%	2.220%
38	5.973	338	340	342	rBV2	1781981	3261184	13.94%	0.636%
39	6.019	342	344	348	rBV3	8179589	21856615	93.40%	4.264%
40	6.087	348	350	351	rVB	2414103	3194762	13.65%	0.623%
41	6.224	358	362	367	rBV4	5452652	16434879	70.23%	3.206%
42	6.304	367	369	374	rBV3	5933827	18590944	79.45%	3.627%
43	6.419	374	379	383	rVV5	4367365	15014725	64.16%	2.929%
44	6.544	385	390	394	rVV3	5764974	22431481	95.86%	4.376%
45	6.613	394	396	403	rVB2	5162341	14626690	62.51%	2.853%
46	6.750	403	408	414	rBV8	4103298	23400323	100.00%	4.565%
47	6.956	422	426	431	rVB5	4739582	17365848	74.21%	3.388%
48	7.196	444	447	451	rBV2	3112405	9869814	42.18%	1.925%
49	10.099	699	701	705	rVB4	4141638	6790017	29.02%	1.325%
50	10.168	705	707	708	rVV	2341285	2916871	12.47%	0.569%
51	10.248	712	714	717	rBV4	2504038	4844881	20.70%	0.945%
52	10.373	723	725	731	rBV6	2442130	7758567	33.16%	1.514%
53	10.488	732	735	737	rVB	4614973	8264067	35.32%	1.612%
54	10.522	737	738	741	rVB3	1527026	2310460	9.87%	0.451%
55	10.591	743	744	747	rVB2	1708257	1922429	8.22%	0.375%
56	10.739	755	757	761	rVB	6251930	11254242	48.09%	2.195%
57	10.899	770	771	773	rVB2	2510602	2015488	8.61%	0.393%
58	10.945	773	775	783	rVB8	1447887	4802418	20.52%	0.937%
59	11.082	783	787	789	rBV2	5178059	8554715	36.56%	1.669%
60	11.139	790	792	793	rBV2	1209173	975953	4.17%	0.190%
61	11.173	793	795	796	rVB2	925341	955796	4.08%	0.186%
62	11.208	796	798	799	rBV2	1624145	2264348	9.68%	0.442%
63	11.265	799	803	805	rVB2	5502127	12203140	52.15%	2.381%
64	11.322	807	808	810	rBV2	1153977	1482770	6.34%	0.289%
65	11.448	816	819	823	rVB6	2761534	7195404	30.75%	1.404%
66	11.528	823	826	827	rBV2	3190766	5051079	21.59%	0.985%
67	11.573	827	830	832	rBV4	3956753	8580513	36.67%	1.674%
68	11.722	839	843	845	rBV2	4611815	10455961	44.68%	2.040%
69	11.813	848	851	853	rVB	4003011	5849824	25.00%	1.141%
70	11.882	855	857	858	rBV	2045384	3738850	15.98%	0.729%
71	12.191	882	884	888	rVB4	4179955	11039326	47.18%	2.154%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121916\
 Data File : BF091803.D
 Acq On : 20 Dec 2016 5:06
 Operator : UM/SJ
 Sample : H6125-03RE
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-47(8-9.5)-12-14-16RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	12.282	888	892	895	rVV4	4168442	10897569	46.57%	2.126%
73	12.374	895	900	902	rVB	6215030	17617835	75.29%	3.437%
74	12.454	904	907	909	rVB	5086536	10187968	43.54%	1.987%
75	12.511	911	912	914	rVB2	2228269	1756667	7.51%	0.343%
76	12.579	914	918	921	rVB3	5297583	13143271	56.17%	2.564%
77	12.636	921	923	926	rBV2	3468326	6999262	29.91%	1.365%
78	12.716	926	930	932	rVB3	2560057	5687638	24.31%	1.110%
79	12.762	932	934	937	rVB4	1520916	2673944	11.43%	0.522%
80	12.819	937	939	940	rBV	842337	710909	3.04%	0.139%
81	12.888	940	945	952	rVB3	7545008	22635818	96.73%	4.416%
82	13.048	955	959	961	rBV2	6362617	12484266	53.35%	2.435%
83	13.174	968	970	971	rBV	1394080	1591988	6.80%	0.311%
84	13.299	977	981	984	rVB3	1513937	3020259	12.91%	0.589%
85	13.357	984	986	987	rVV	1628206	1886208	8.06%	0.368%
86	13.391	987	989	990	rVV	1340247	1588157	6.79%	0.310%
87	13.459	993	995	997	rVV3	674275	952569	4.07%	0.186%
88	13.528	999	1001	1003	rBV	848641	780945	3.34%	0.152%
89	13.905	1032	1034	1035	rBV	788803	1517980	6.49%	0.296%
90	15.322	1155	1158	1162	rBV	908446	1304727	5.58%	0.255%


Sum of corrected areas: 512613934

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121916\
Data File : BF091803.D
Acq On : 20 Dec 2016 5:06
Operator : UM/SJ
Sample : H6125-03RE
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-47(8-9.5)-12-14-16RE

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

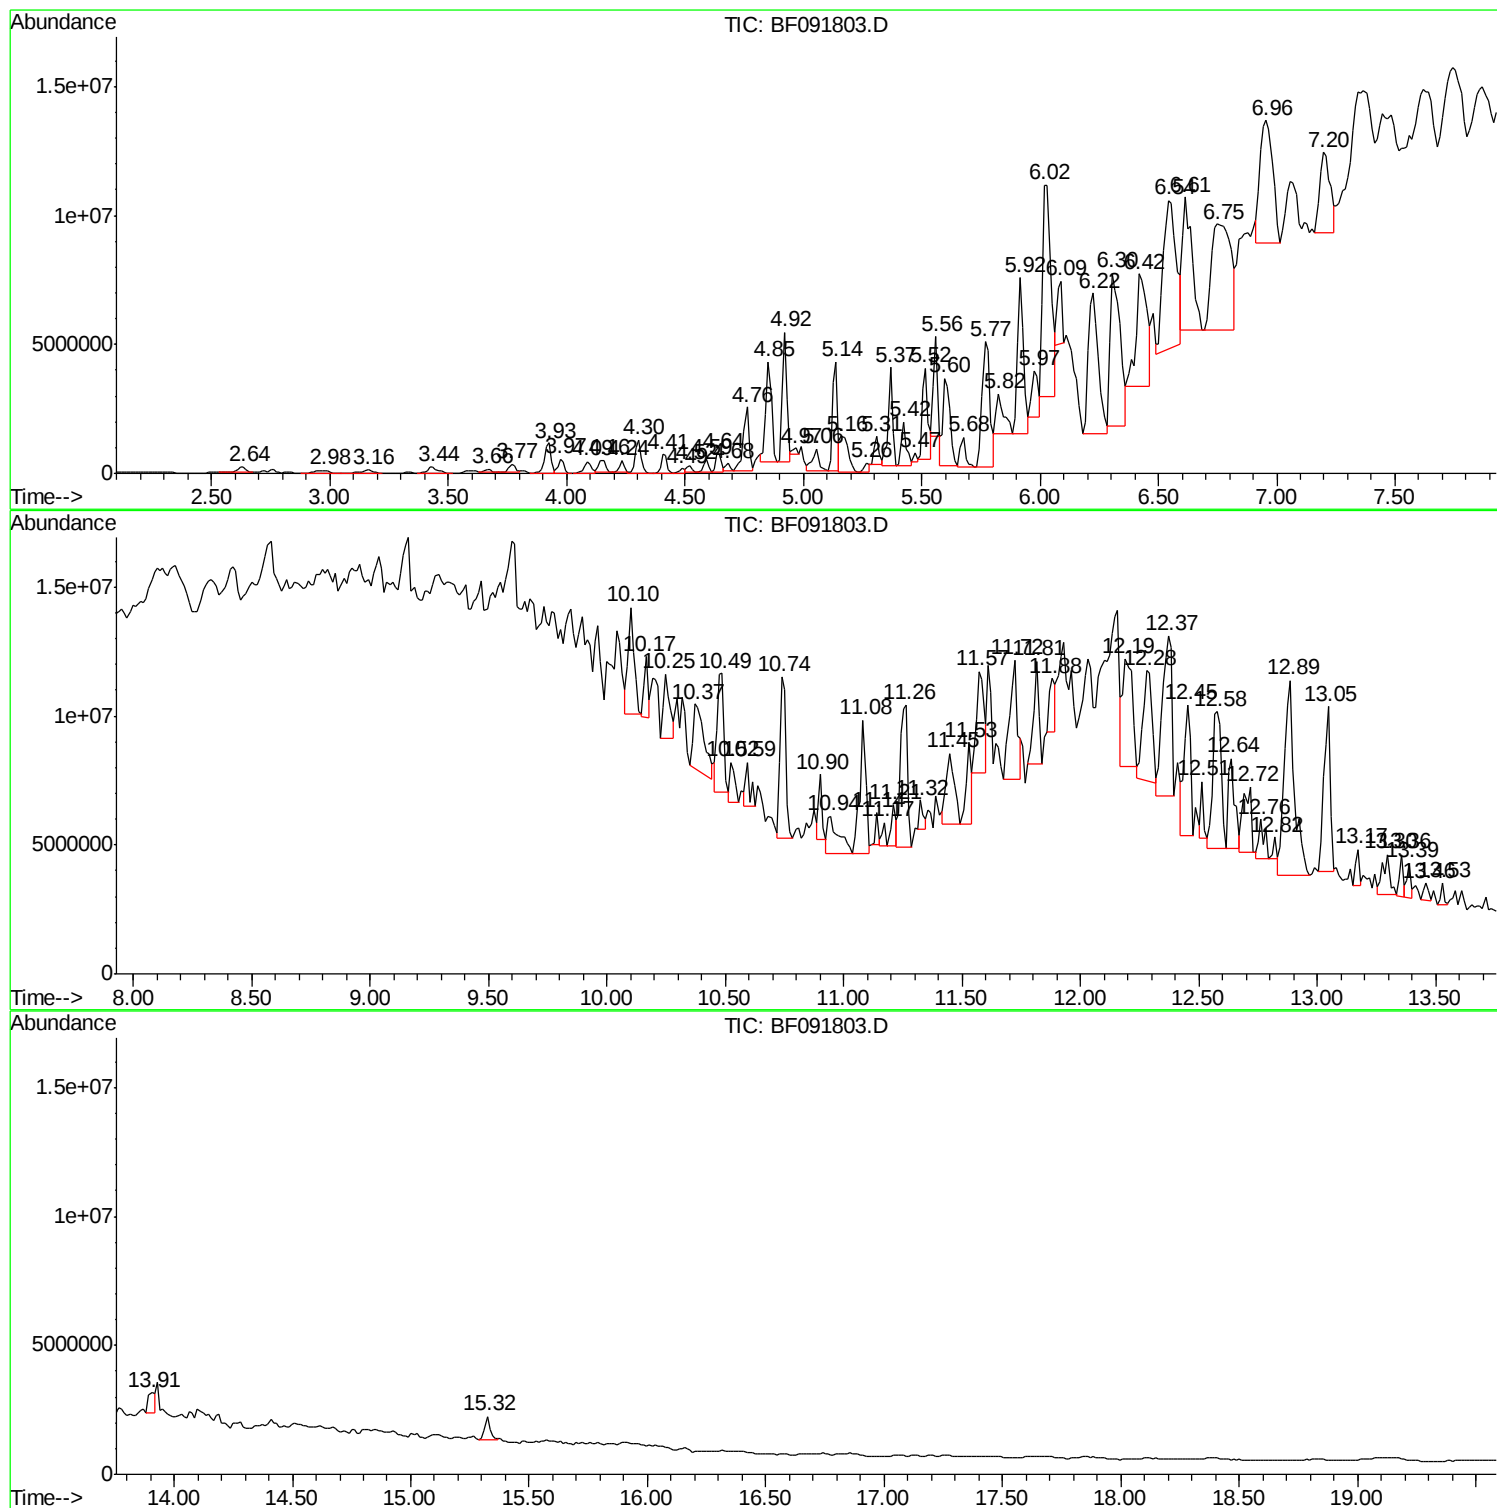

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF121916\
Data_File : BF091803.D
Acq_On : 20-Dec-2016 5:066
Operator : UM/SJJ
Sample : H6125-03REE
Misc :
ALS_Vial : 23 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SB-47(8-9.5)-12-14-16RE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
