

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121916\
 Data File : BF091804.D
 Acq On : 20 Dec 2016 5:34
 Operator : UM/SJ
 Sample : H6125-05RE
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-45(8-9)-12-14-16RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.647	40	49	52	rVB	196669	482414	2.31%	0.084%
2	2.990	70	79	85	rVB2	77425	290478	1.39%	0.050%
3	3.173	85	95	101	rBV3	114118	331382	1.59%	0.058%
4	3.447	113	119	126	rVB	201322	566751	2.72%	0.098%
5	3.618	126	134	136	rBV2	77956	270641	1.30%	0.047%
6	3.675	136	139	142	rVB	123664	228004	1.09%	0.040%
7	3.778	142	148	151	rBV	301033	559680	2.68%	0.097%
8	3.927	155	161	164	rBV2	1080168	2167977	10.40%	0.377%
9	3.984	164	166	169	rVB	517575	740075	3.55%	0.129%
10	4.098	169	176	178	rBV2	410376	822558	3.95%	0.143%
11	4.156	178	181	185	rVB	386440	762151	3.66%	0.132%
12	4.304	191	194	200	rVB2	1080649	1795410	8.61%	0.312%
13	4.418	200	204	207	rVB	648108	917286	4.40%	0.159%
14	4.521	211	213	216	rVB2	208320	320027	1.54%	0.056%
15	4.590	216	219	221	rBV2	360673	565313	2.71%	0.098%
16	4.647	221	224	226	rBV	675521	887021	4.25%	0.154%
17	4.681	226	227	229	rVB2	197421	218499	1.05%	0.038%
18	4.761	229	234	236	rBV	2283029	3366482	16.15%	0.585%
19	4.853	239	242	246	rVB2	3485156	5926380	28.43%	1.030%
20	4.921	246	248	251	rBV2	4741395	6748499	32.37%	1.172%
21	5.058	256	260	264	rVB	868370	1354871	6.50%	0.235%
22	5.138	264	267	268	rBV	4334294	5634428	27.03%	0.979%
23	5.161	268	269	276	rVB3	1241914	2919904	14.01%	0.507%
24	5.264	276	278	279	rBV	332142	422440	2.03%	0.073%
25	5.310	279	282	284	rBV2	1113870	1644813	7.89%	0.286%
26	5.367	284	287	289	rVB	3562690	5073538	24.34%	0.881%
27	5.424	289	292	295	rBV3	1657065	2257553	10.83%	0.392%
28	5.470	295	296	297	rBV	363195	356801	1.71%	0.062%
29	5.516	297	300	302	rBV	3396098	5420342	26.00%	0.942%
30	5.561	302	304	305	rVB	3753124	3802438	18.24%	0.661%
31	5.596	305	307	312	rVB2	3064154	6562663	31.48%	1.140%
32	5.676	312	314	318	rVB	1189271	1635667	7.85%	0.284%
33	5.767	318	322	325	rBV2	4569114	10055231	48.23%	1.747%
34	5.824	325	327	332	rVB4	1623523	3871314	18.57%	0.673%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121916\
 Data File : BF091804.D
 Acq On : 20 Dec 2016 5:34
 Operator : UM/SJ
 Sample : H6125-05RE
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-45(8-9)-12-14-16RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	5.916	332	335	338	rBV2	5835198	10192790	48.89%	1.771%
36	5.973	338	340	342	rBV2	1906654	3291411	15.79%	0.572%
37	6.019	342	344	348	rBV3	8365946	20847437	100.00%	3.622%
38	6.076	348	349	358	rVB4	5896402	19991735	95.90%	3.473%
39	6.213	358	361	367	rBV4	4773587	15034019	72.11%	2.612%
40	6.304	367	369	374	rBV3	5404540	15916884	76.35%	2.765%
41	6.384	374	376	377	rBV2	1347800	2138663	10.26%	0.372%
42	6.419	377	379	383	rBV3	3342015	8434363	40.46%	1.465%
43	6.544	385	390	393	rBV3	5235040	18512580	88.80%	3.216%
44	6.613	393	396	403	rVB	5579851	17538198	84.13%	3.047%
45	6.773	403	410	411	rBV5	4032705	16189741	77.66%	2.813%
46	6.944	422	425	431	rVB5	4761494	17791758	85.34%	3.091%
47	7.059	432	435	441	rBV6	2514129	7934441	38.06%	1.378%
48	7.207	444	448	452	rBV5	3226375	11193879	53.69%	1.945%
49	10.099	699	701	705	rVB3	4158570	6628817	31.80%	1.152%
50	10.168	705	707	708	rVV	2459164	3015529	14.46%	0.524%
51	10.248	712	714	717	rBV4	2165527	3992377	19.15%	0.694%
52	10.385	723	726	732	rVV7	2309073	8206190	39.36%	1.426%
53	10.488	732	735	737	rVV	5447321	8840266	42.40%	1.536%
54	10.522	737	738	741	rVB3	1613765	2439631	11.70%	0.424%
55	10.739	755	757	760	rVB	6533262	10678317	51.22%	1.855%
56	10.899	770	771	773	rVB2	1996735	1824404	8.75%	0.317%
57	10.945	773	775	783	rVB8	1500845	3793001	18.19%	0.659%
58	11.082	783	787	789	rBV2	4100965	5760795	27.63%	1.001%
59	11.139	790	792	793	rBV	809298	699056	3.35%	0.121%
60	11.196	795	797	799	rVB	1778955	2335130	11.20%	0.406%
61	11.253	799	802	804	rVB2	3980773	7181430	34.45%	1.248%
62	11.322	804	808	810	rBV3	1326366	3443318	16.52%	0.598%
63	11.391	812	814	815	rBV	1021066	1003623	4.81%	0.174%
64	11.448	815	819	822	rVV5	1913973	5319165	25.51%	0.924%
65	11.516	823	825	827	rVV2	2242636	3839363	18.42%	0.667%
66	11.562	827	829	831	rVV3	5392008	10394297	49.86%	1.806%
67	11.596	831	832	834	rVV	5541020	7467256	35.82%	1.297%
68	11.642	834	836	838	rVV2	2308655	4579905	21.97%	0.796%
69	11.711	838	842	843	rVV2	6522784	13480725	64.66%	2.342%
70	11.802	847	850	852	rVV	6092450	11027030	52.89%	1.916%
71	11.859	852	855	856	rVV2	5348530	10406345	49.92%	1.808%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121916\
 Data File : BF091804.D
 Acq On : 20 Dec 2016 5:34
 Operator : UM/SJ
 Sample : H6125-05RE
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-45(8-9)-12-14-16RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	11.905	856	859	861	rVV2	7352013	19588202	93.96%	3.403%
73	12.008	865	868	870	rVV2	6626956	17344141	83.20%	3.013%
74	12.065	870	873	874	rVV2	6081410	14920321	71.57%	2.592%
75	12.122	876	878	880	rVV3	8348836	15676302	75.20%	2.723%
76	12.179	880	883	886	rVV4	6698855	17384248	83.39%	3.020%
77	12.259	887	890	894	rVV5	6140657	14813288	71.06%	2.573%
78	12.351	894	898	900	rVV	7344913	19688803	94.44%	3.420%
79	12.385	900	901	903	rVV2	1844414	2852786	13.68%	0.496%
80	12.442	903	906	907	rVV	4192876	7354041	35.28%	1.278%
81	12.488	907	910	912	rVB4	1266009	2263851	10.86%	0.393%
82	12.568	914	917	919	rVV3	5197791	8874567	42.57%	1.542%
83	12.614	920	921	922	rVV	2926868	2286476	10.97%	0.397%
84	12.694	925	928	930	rVB3	1484644	3296299	15.81%	0.573%
85	12.865	939	943	946	rBV	5948832	13842959	66.40%	2.405%
86	13.025	954	957	960	rVV2	4057325	8104828	38.88%	1.408%
87	13.128	964	966	968	rBV3	678185	836348	4.01%	0.145%
88	13.162	968	969	971	rVB2	1202611	1060048	5.08%	0.184%
89	13.345	984	985	987	rBV	1097383	1181494	5.67%	0.205%
90	13.379	987	988	990	rVV2	702033	725069	3.48%	0.126%
91	13.528	999	1001	1002	rVB	475860	628806	3.02%	0.109%
92	13.608	1006	1008	1011	rVB2	579739	655171	3.14%	0.114%
93	13.928	1034	1036	1037	rVB	696038	796469	3.82%	0.138%
94	15.322	1156	1158	1162	rVB	858352	1097812	5.27%	0.191%


Sum of corrected areas: 575615229

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121916\
Data File : BF091804.D
Acq On : 20 Dec 2016 5:34
Operator : UM/SJ
Sample : H6125-05RE
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-45(8-9)-12-14-16RE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

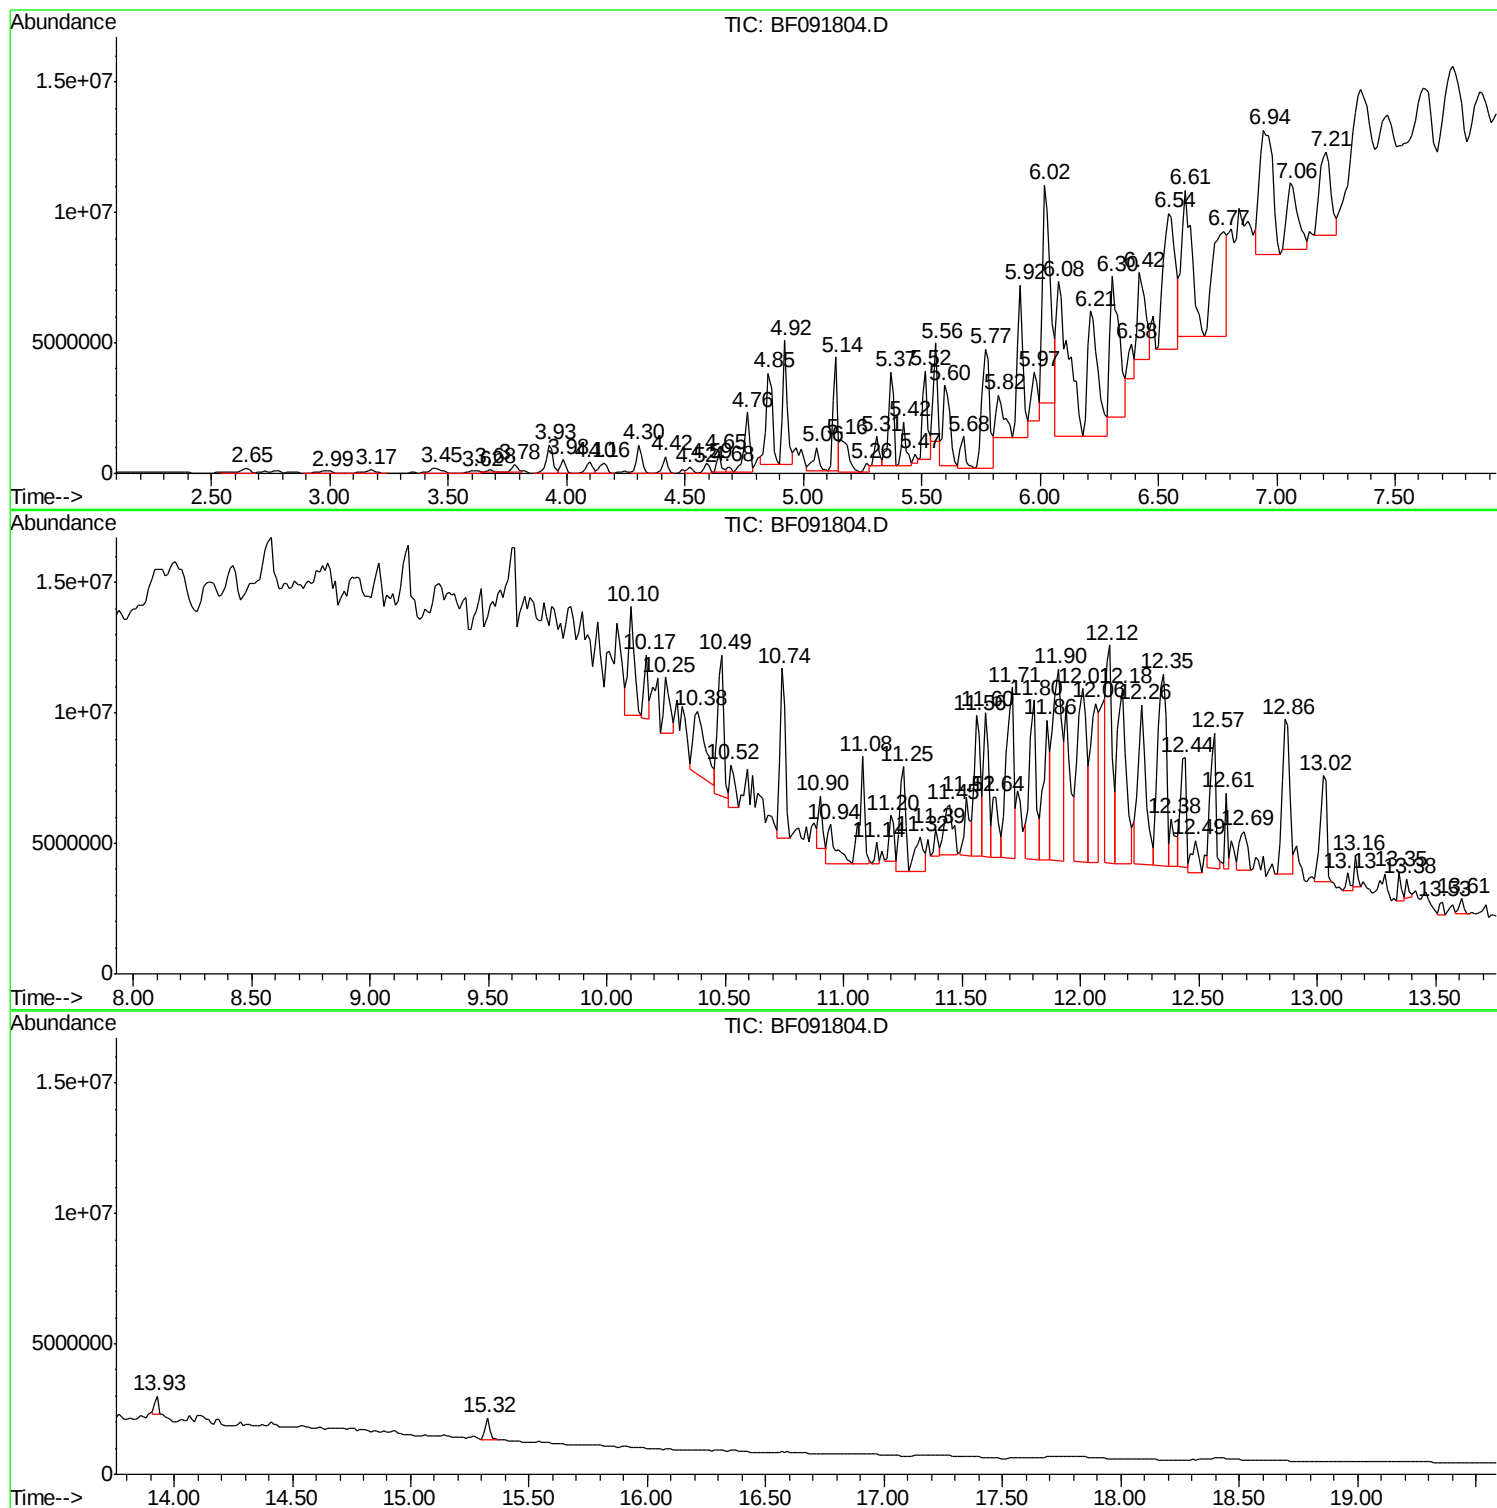

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF121916\
Data_File : BF091804.D
Acq_On : 20-Dec-2016 5:344
Operator : UM/SJJ
Sample : H6125-05REE
Misc :
ALS_Vial : 24 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SB-45(8-9)-12-14-16RE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
