


Data Path : Z:\HPCHEM1\BNA F\DATA\BF121916\
 Data File : BF091778.D
 Acq On : 19 Dec 2016 14:10
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 17 22:53:54 2016

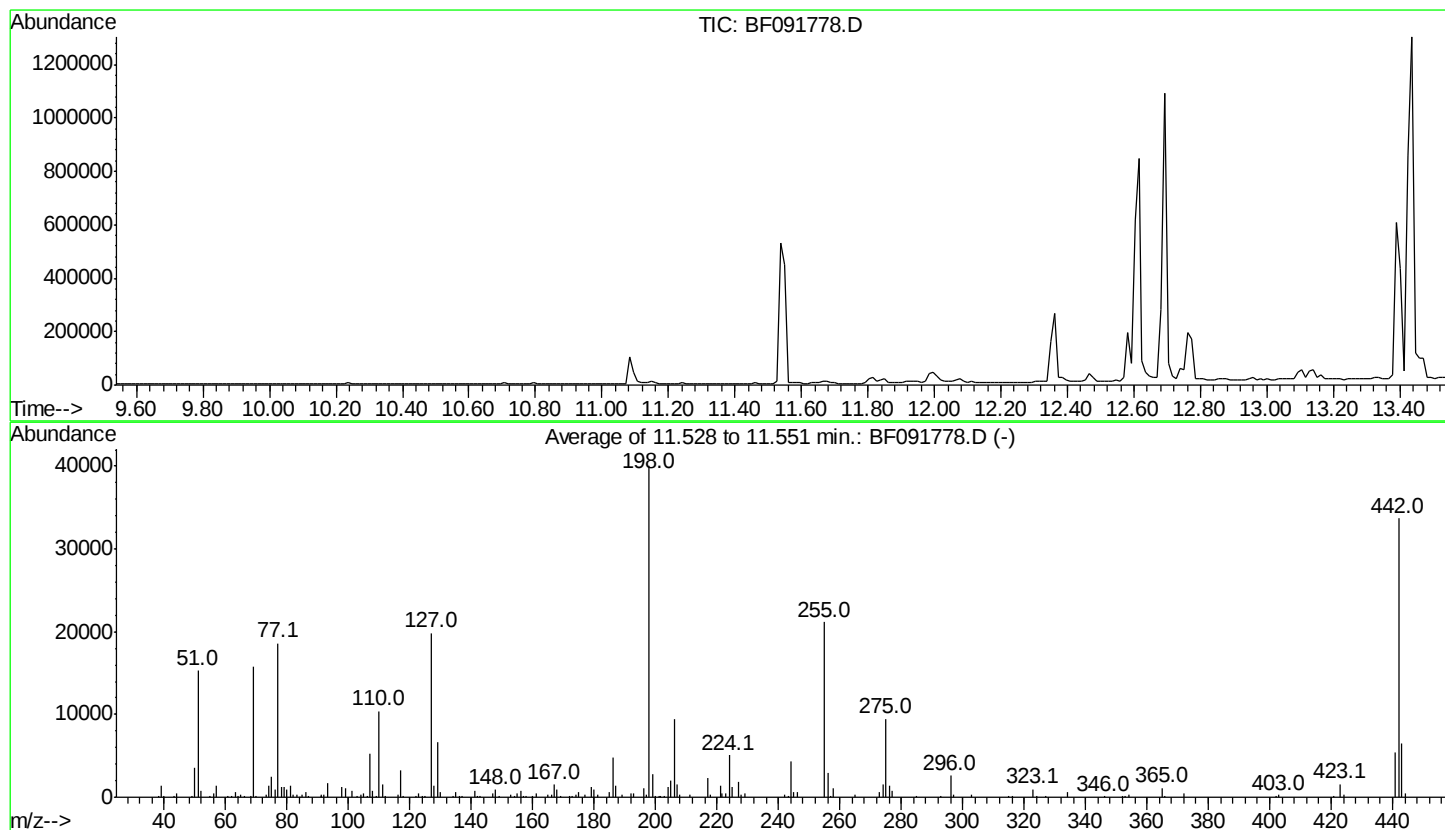

AutoFind: Scans 826, 827, 828; Background Corrected with Scan 823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	15311	PASS
68	69	0.00	2	1.1	180	PASS
69	198	0.00	100	39.5	15819	PASS
70	69	0.00	2	0.7	116	PASS
127	198	10	80	49.5	19824	PASS
197	198	0.00	2	0.6	245	PASS
198	198	100	100	100.0	40074	PASS
199	198	5	9	7.1	2853	PASS
275	198	10	60	23.6	9438	PASS
365	198	1	100	2.8	1136	PASS
441	442	0.01	24	15.9	5354	PASS
442	198	50	100	84.0	33682	PASS
443	442	15	24	19.2	6475	PASS