
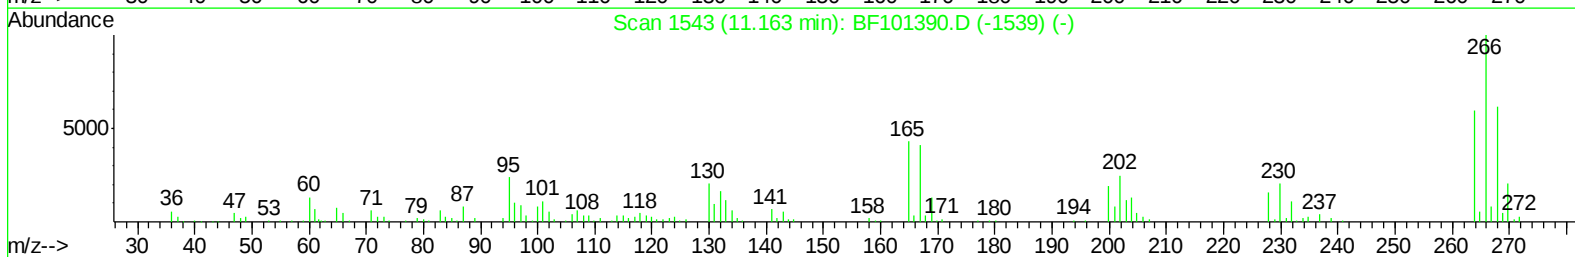
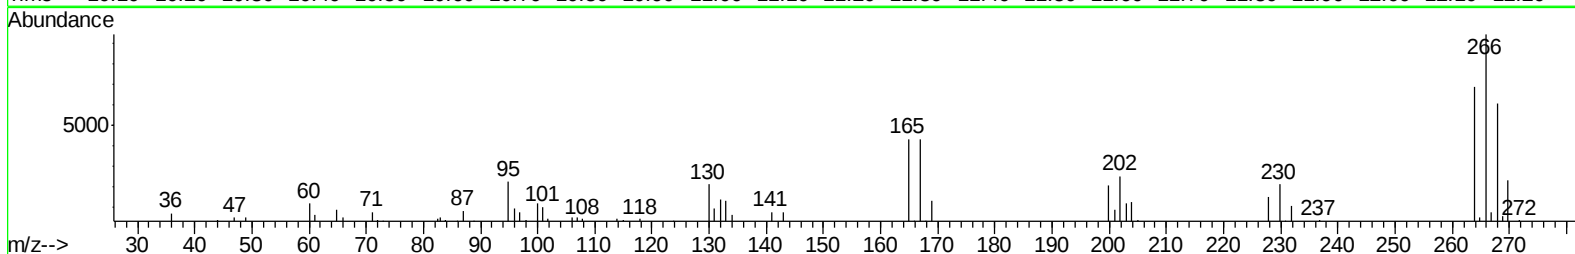


Data Path : Z:\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101541.D
Acq On : 20 Dec 2017 00:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 08:13:19 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 18 15:38:59 2017
Response via : Initial Calibration

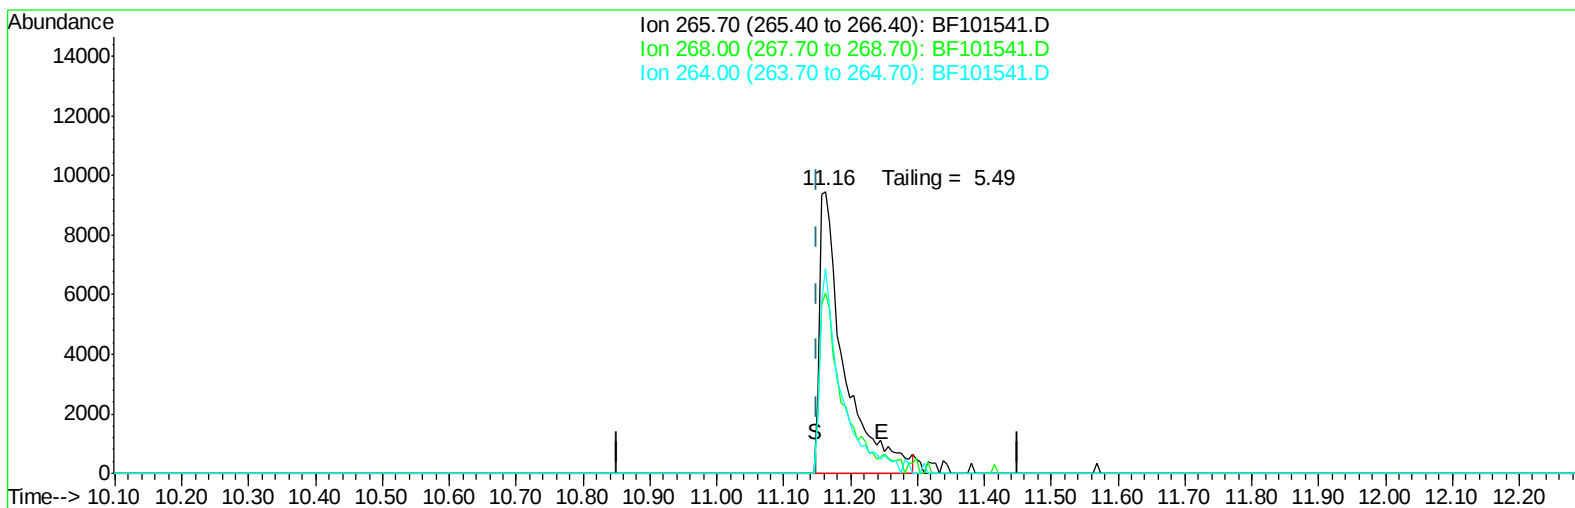

TIC: BF101541.D

(69) Pentachlorophenol (C)

11.163min (+0.012) 28179.09ng

response 23984

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.10
264.00	61.90	72.96
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA F\DATA\BF121917\  
Data File : BF101541.D  
Acq On    : 20 Dec 2017  00:39  
Operator  : SJ/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Data File : BF101541.D

Acq On : 20 Dec 2017 00:39

Operator : SJ/JU

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1


Quant Time: Dec 20 08:13:19 2017

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Dec 18 15:38:59 2017

Response via : Initial Calibration

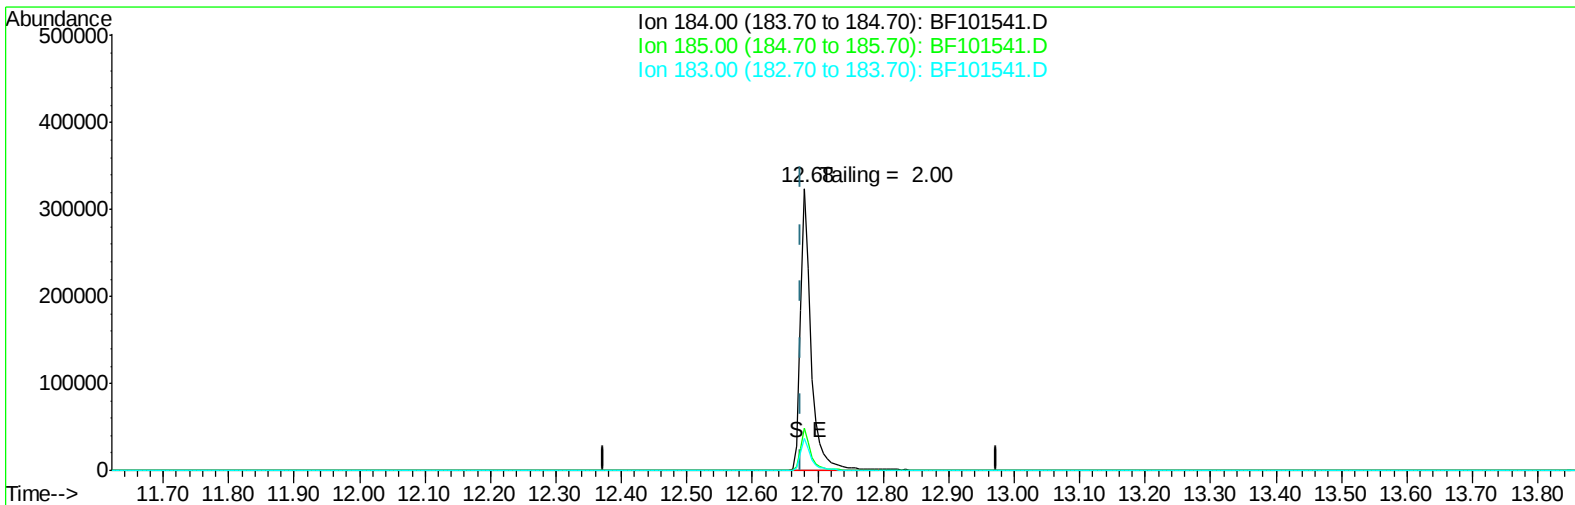

lon 184.00 (183.70 to 184.70): BF101541.D

Ion 185.00 (184.70 to 185.70): BF101541.D

Ion 183.00 (182.70 to 183.70): BF101541.D


12.68 Bailing = 2.00

.68 Bailing = 2.00


\$

~~E~~

Time--> 11.70 11.80 11.90 12.00 12.10 12.20 12.30 12.40 12.50 12.60 12.70 12.80 12.90 13.00 13.10 13.20 13.30 13.40 13.50 13.60 13.70 13.80

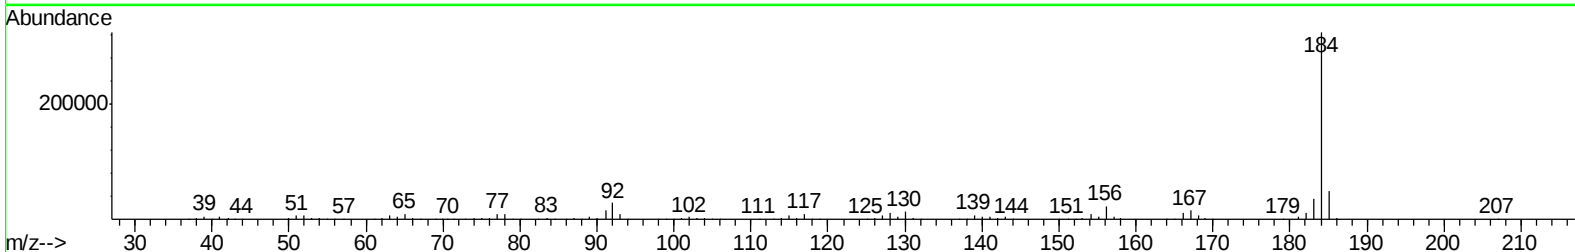

m/z--> 30 40 50 60 70 80 90 100 110 120 130 140 150 160 170 180 190 200 210

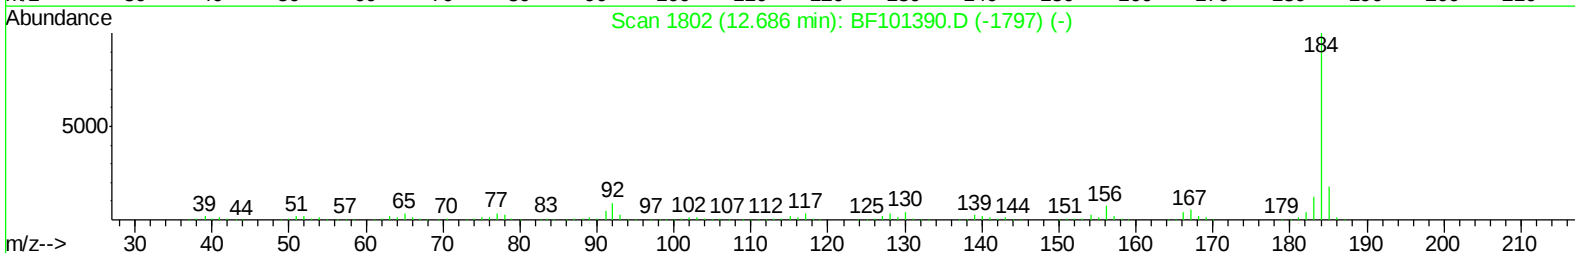

Scan 1802 (12.686 min): BF101390.D (-1797) (-)

m/z--> 30 40 50 60 70 80 90 100 110 120 130 140 150 160 170 180 190 200 210

TIC: BF101541.D

(76) Benzidine

12.680min (+0.006) 66781.66ng

response 369490

Ion	Exp%	Act%
-----	------	------

184.00	100	100
--------	-----	-----

185.00	15.70	14.96
--------	-------	-------

183.00	11.60	11.41
--------	-------	-------

0.00 0.00 0.00