
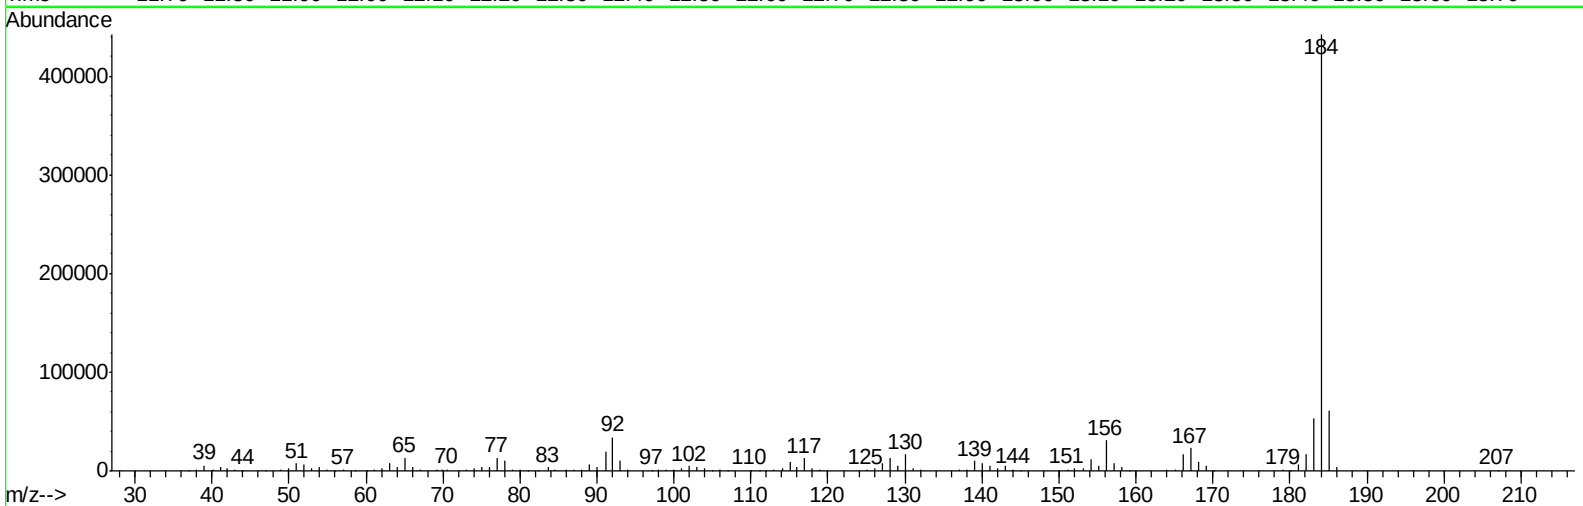


```
Data Path : Z:\HPCHEM1\BNA F\DATA\BF121917\  
Data File : BF101516.D  
Acq On    : 19 Dec 2017  11:19  
Operator  : SJ/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Dec 20 08:31:46 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 18 15:38:59 2017
Response via : Initial Calibration

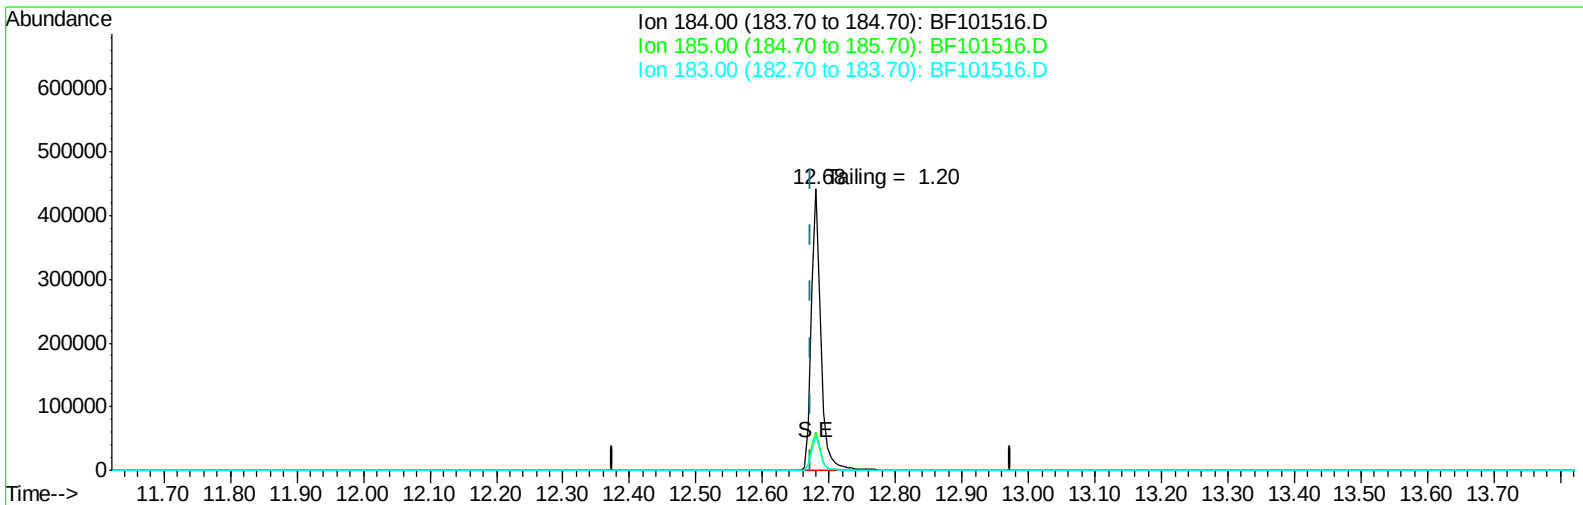

TIC: BF101516.D

(76) Benzidine



12.680min (+0.006) 0.00ng

response 448604

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.78
183.00	11.60	12.07
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101516.D
Acq On : 19 Dec 2017 11:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 08:31:46 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 18 15:38:59 2017
Response via : Initial Calibration

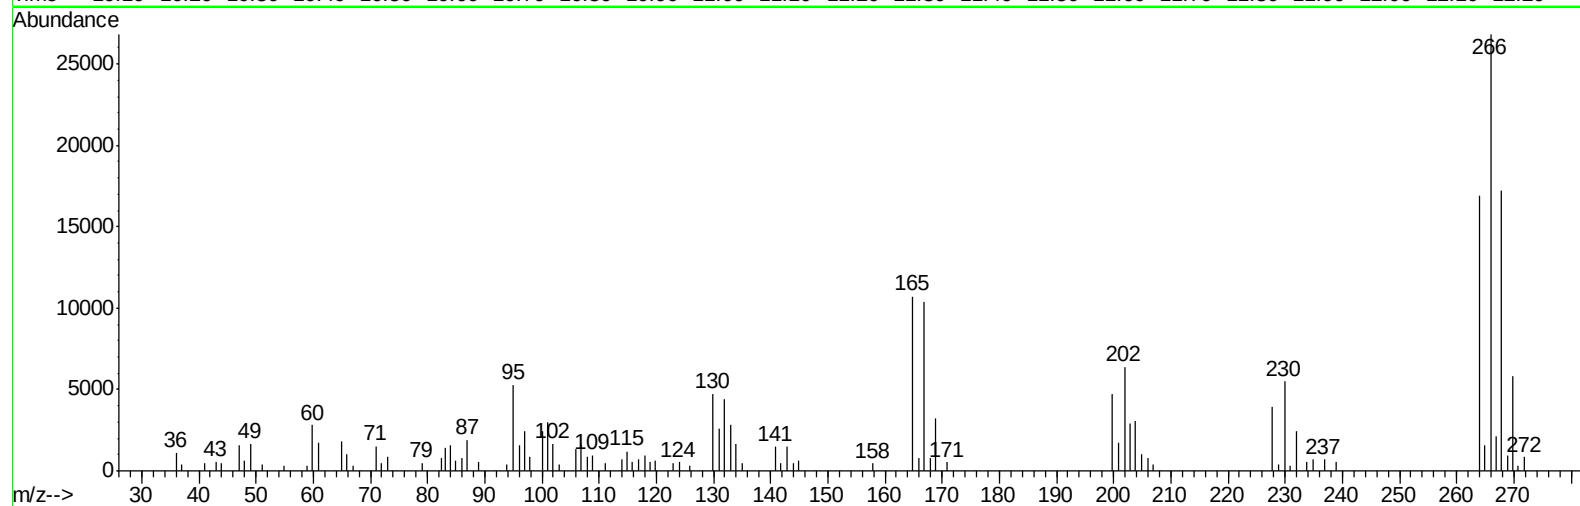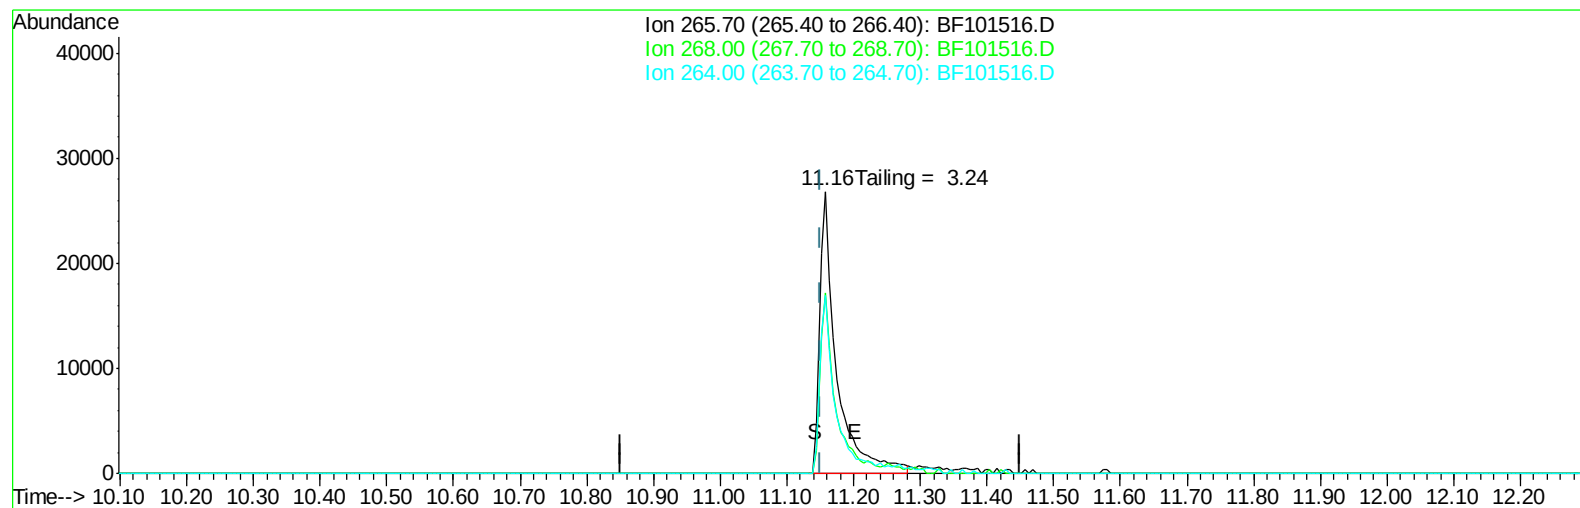

TIC: BF101516.D

(69) Pentachlorophenol (C)

11.157min (+0.006) 30047.26ng

response 46609

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.20
264.00	61.90	63.10
0.00	0.00	0.00