

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121917\
 Data File : BF101530.D
 Acq On : 19 Dec 2017 18:48
 Operator : SJ/JU
 Sample : I6958-01 50X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DRUM-1-4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	572	577	582	rBV3	9498	19956	1.85%	0.349%
2	6.510	746	752	766	rBV4	11276	40900	3.79%	0.715%
3	6.610	766	769	777	rVV	21140	39565	3.66%	0.691%
4	6.810	799	803	821	rBV	639677	739566	68.45%	12.922%
5	6.969	827	830	838	rBV	32781	44446	4.11%	0.777%
6	7.416	900	906	913	rBV2	9921	23461	2.17%	0.410%
7	8.092	1017	1021	1049	rBV	832283	1030348	95.36%	18.002%
8	9.175	1201	1205	1220	rBV	46387	69709	6.45%	1.218%
9	9.845	1315	1319	1333	rBV	1032587	1080500	100.00%	18.878%
10	11.339	1569	1573	1589	rBV	929673	1068513	98.89%	18.669%
11	12.921	1839	1842	1847	rBV	55082	50089	4.64%	0.875%
12	13.986	2019	2023	2035	rBV	622350	720978	66.73%	12.597%
13	15.462	2268	2274	2285	rVB	523459	795477	73.62%	13.898%


Sum of corrected areas: 5723508

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101530.D
Acq On : 19 Dec 2017 18:48
Operator : SJ/JU
Sample : I6958-01 50X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DRUM-1-4

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

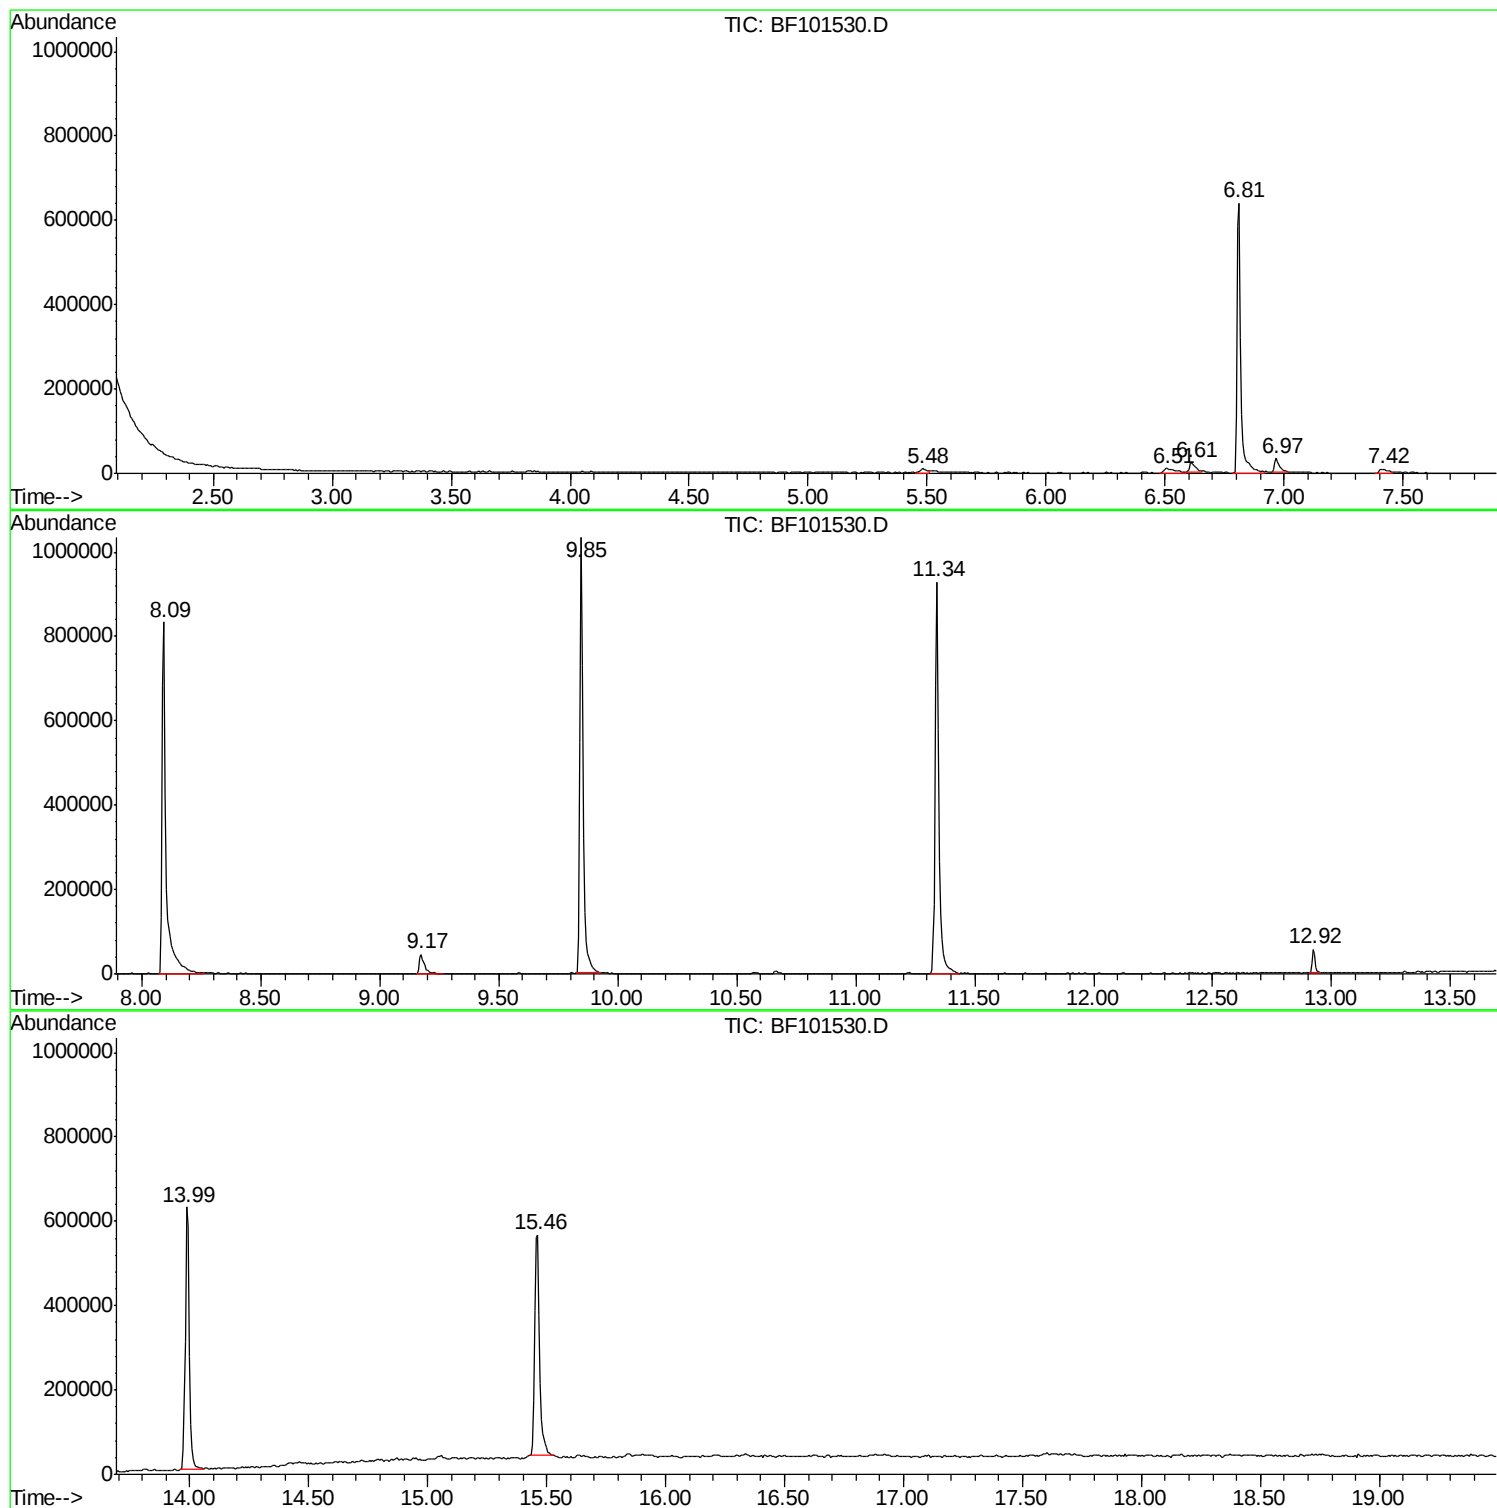

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121917\
Data_File : BF101530.D
Acq_On : 19-Dec-2017 18:488
Operator : SJ/JUU
Sample : I6958-01_50XX
Misc :
ALS_Vial : 15 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
DRUM-1-4

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
