

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121917\
 Data File : BF101531.D
 Acq On : 19 Dec 2017 19:15
 Operator : SJ/JU
 Sample : I6676-08 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-01-121817

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.016	495	498	507	rBV	32232	56595	6.44%	0.601%
2	5.434	566	569	587	rBV	338198	601288	68.38%	6.382%
3	6.451	739	742	761	rBV	321447	628096	71.43%	6.666%
4	6.581	761	764	776	rVB	591066	649359	73.85%	6.892%
5	6.810	799	803	810	rBV	683286	704476	80.12%	7.477%
6	6.963	825	829	839	rBV	505958	502013	57.09%	5.328%
7	7.380	897	900	917	rBV	239927	380534	43.28%	4.039%
8	8.092	1017	1021	1042	rBV	729593	879329	100.00%	9.333%
9	9.163	1200	1203	1213	rBV	561997	625798	71.17%	6.642%
10	9.233	1213	1215	1219	rVB3	10377	13003	1.48%	0.138%
11	9.569	1265	1272	1278	rVB2	12384	23795	2.71%	0.253%
12	9.845	1315	1319	1333	rVV2	757455	788125	89.63%	8.365%
13	10.263	1387	1390	1393	rVB	15948	12334	1.40%	0.131%
14	10.645	1452	1455	1467	rVB	180085	230658	26.23%	2.448%
15	10.733	1467	1470	1477	rBV2	20016	25482	2.90%	0.270%
16	11.186	1544	1547	1549	rBV	10346	9369	1.07%	0.099%
17	11.339	1569	1573	1586	rBV	637431	675115	76.78%	7.166%
18	11.963	1675	1679	1685	rBV8	5735	10942	1.24%	0.116%
19	12.398	1749	1753	1760	rBV5	14526	20116	2.29%	0.214%
20	12.557	1777	1780	1788	rVB	42583	45792	5.21%	0.486%
21	12.792	1814	1820	1825	rBV	41699	55094	6.27%	0.585%
22	12.915	1838	1841	1848	rVB	457266	405814	46.15%	4.307%
23	13.127	1868	1877	1880	rBV2	13697	26364	3.00%	0.280%
24	13.180	1884	1886	1889	rBV	7435	8877	1.01%	0.094%
25	13.468	1932	1935	1938	rBV	8977	11176	1.27%	0.119%
26	13.745	1980	1982	1985	rBV4	8439	10728	1.22%	0.114%
27	13.804	1987	1992	1996	rVV6	22703	34754	3.95%	0.369%
28	13.986	2018	2023	2034	rBV	761535	858442	97.62%	9.111%
29	14.157	2050	2052	2059	rVB7	12231	14395	1.64%	0.153%
30	14.215	2059	2062	2066	rBV4	11989	17590	2.00%	0.187%
31	14.421	2095	2097	2100	rVV4	16046	15558	1.77%	0.165%
32	14.721	2146	2148	2152	rVB3	19965	20186	2.30%	0.214%
33	15.033	2198	2201	2203	rBV	49824	70651	8.03%	0.750%
34	15.333	2249	2252	2255	rBV	36904	46439	5.28%	0.493%

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101531.D
Acq On : 19 Dec 2017 19:15
Operator : SJ/JU
Sample : I6676-08 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-121817

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.398	2260	2263	2266	rVV	47971	65049	7.40%	0.690%
36	15.456	2269	2273	2284	rVB2	595521	852190	96.91%	9.045%
37	15.845	2337	2339	2344	rVB3	23715	26199	2.98%	0.278%


Sum of corrected areas: 9421725

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101531.D
Acq On : 19 Dec 2017 19:15
Operator : SJ/JU
Sample : I6676-08 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
OK-01-121817

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

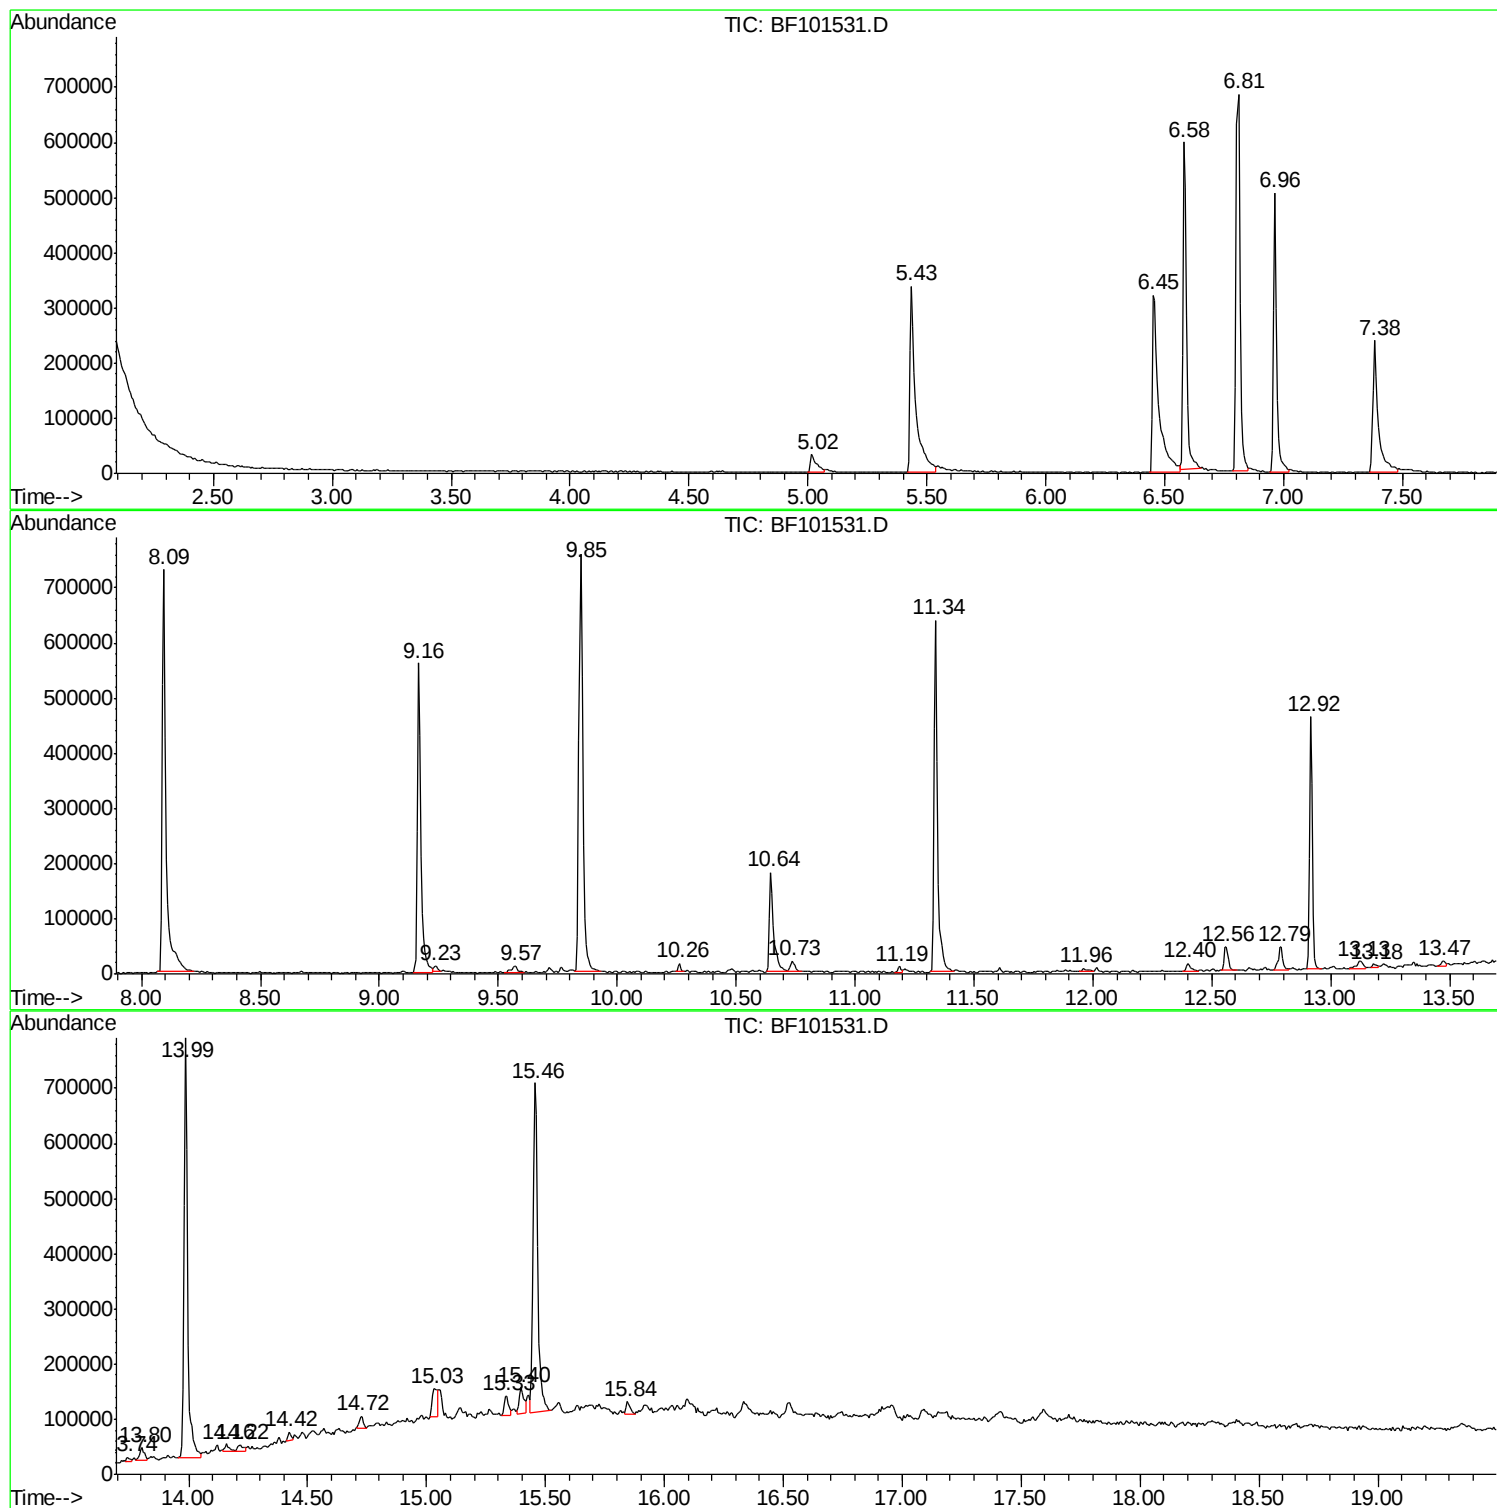

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101531.D
Acq On : 19 Dec 2017 19:15
Operator : SJ/JU
Sample : I6676-08 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-121817










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.58 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.58	18.44 ng	649359	1,4-Dichlorobenzene-d4	6.81

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

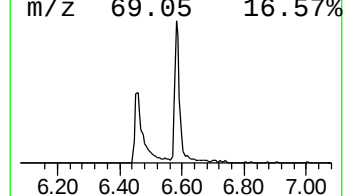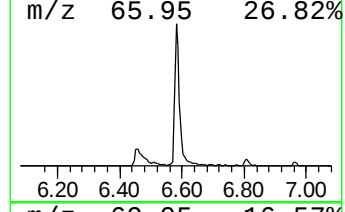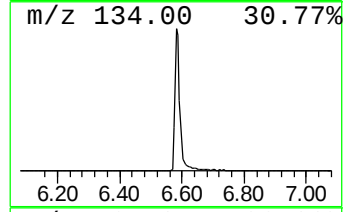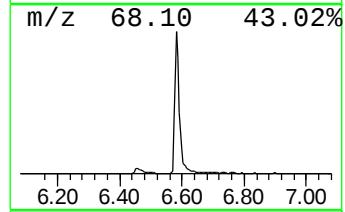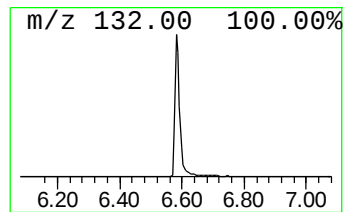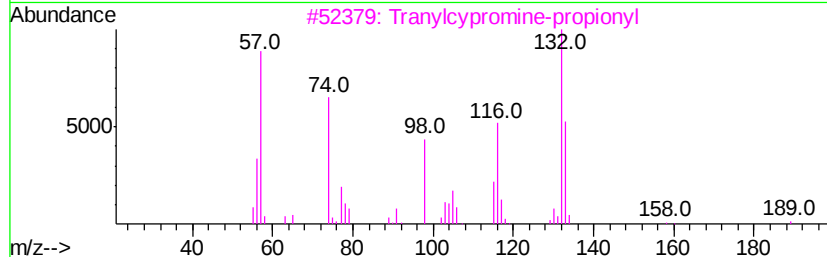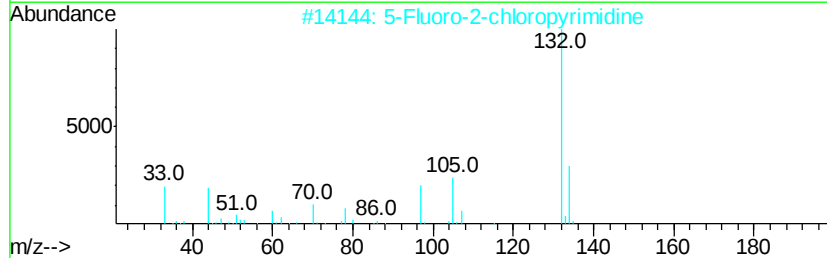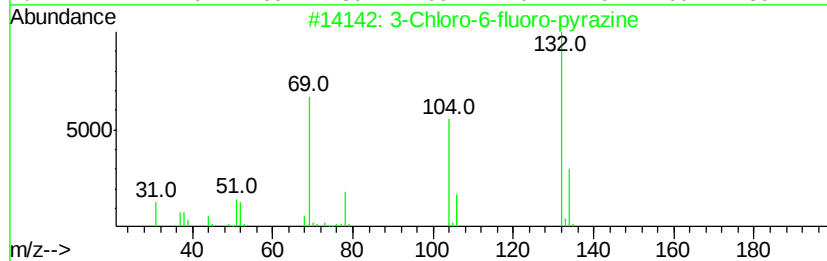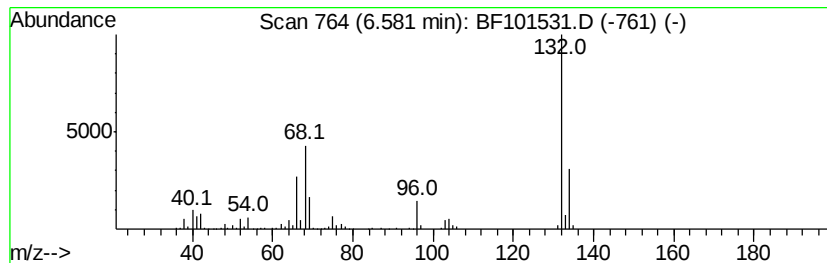

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121917\
Data File : BF101531.D
Acq On : 19 Dec 2017 19:15
Operator : SJ/JU
Sample : I6676-08 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-121817

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.58	6.58	18.4	ng	649359	1	6.81	704476	20.0