

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121917\
 Data File : BF101535.D
 Acq On : 19 Dec 2017 21:03
 Operator : SJ/JU
 Sample : I6981-01 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PHMHA-WCS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.022	495	499	509	rBV	17454	34350	2.76%	0.328%
2	5.440	566	570	592	rBV	145894	308171	24.77%	2.941%
3	6.457	740	743	758	rBV	162101	349603	28.10%	3.337%
4	6.587	762	765	779	rVB	307701	379223	30.48%	3.619%
5	6.804	799	802	818	rBV	906080	936459	75.27%	8.938%
6	6.963	826	829	844	rVB	275657	296535	23.84%	2.830%
7	7.386	898	901	915	rBV	116825	212540	17.08%	2.029%
8	8.092	1017	1021	1040	rBV	1060001	1244099	100.00%	11.874%
9	9.163	1200	1203	1213	rBV	347037	386533	31.07%	3.689%
10	9.710	1291	1296	1299	rBV3	8849	13850	1.11%	0.132%
11	9.845	1315	1319	1324	rBV2	1158155	1129237	90.77%	10.778%
12	10.057	1351	1355	1358	rBV3	10524	16599	1.33%	0.158%
13	10.092	1358	1361	1365	rVB4	9760	13024	1.05%	0.124%
14	10.263	1383	1390	1393	rBV3	21601	24967	2.01%	0.238%
15	10.404	1407	1414	1420	rVB7	12957	29043	2.33%	0.277%
16	10.480	1420	1427	1429	rBV3	17440	29036	2.33%	0.277%
17	10.510	1429	1432	1435	rVB	25023	20377	1.64%	0.194%
18	10.651	1451	1456	1459	rBV2	56877	69349	5.57%	0.662%
19	10.680	1459	1461	1465	rVV	19143	20881	1.68%	0.199%
20	10.739	1467	1471	1479	rVB4	26996	45839	3.68%	0.438%
21	10.869	1490	1493	1496	rBV2	14542	13371	1.07%	0.128%
22	11.186	1544	1547	1549	rBV3	18179	15661	1.26%	0.149%
23	11.339	1569	1573	1575	rBV	988732	942286	75.74%	8.994%
24	11.363	1575	1577	1583	rVV	188830	194587	15.64%	1.857%
25	11.421	1583	1587	1593	rVB	41047	45590	3.66%	0.435%
26	11.610	1617	1619	1621	rVB	17336	13503	1.09%	0.129%
27	11.845	1655	1659	1661	rBV	23292	26732	2.15%	0.255%
28	11.874	1661	1664	1667	rVB	27342	25567	2.06%	0.244%
29	11.957	1675	1678	1680	rBV	36473	41889	3.37%	0.400%
30	11.980	1680	1682	1686	rVB	20783	19490	1.57%	0.186%
31	12.139	1706	1709	1712	rBV	18343	21984	1.77%	0.210%
32	12.186	1712	1717	1720	rVV6	11792	13931	1.12%	0.133%
33	12.392	1749	1752	1757	rBV2	29242	48475	3.90%	0.463%
34	12.492	1765	1769	1776	rVB5	15464	29255	2.35%	0.279%

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
 Data File : BF101535.D
 Acq On : 19 Dec 2017 21:03
 Operator : SJ/JU
 Sample : I6981-01 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PHMHA-WCS

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.557	1776	1780	1785	rBV	328109	309079	24.84%	2.950%
36	12.710	1803	1806	1813	rBV3	19986	30344	2.44%	0.290%
37	12.786	1813	1819	1825	rBV	266134	320389	25.75%	3.058%
38	12.839	1825	1828	1834	rVB6	22537	23635	1.90%	0.226%
39	12.916	1838	1841	1845	rVB	306680	275325	22.13%	2.628%
40	13.010	1852	1857	1859	rBV3	18055	29893	2.40%	0.285%
41	13.057	1862	1865	1868	rBV5	19142	20280	1.63%	0.194%
42	13.092	1868	1871	1872	rBV3	17841	16820	1.35%	0.161%
43	13.221	1891	1893	1897	rVB2	21245	17417	1.40%	0.166%
44	13.315	1906	1909	1912	rBV	21847	26648	2.14%	0.254%
45	13.474	1934	1936	1939	rVB	21650	14229	1.14%	0.136%
46	13.639	1961	1964	1967	rBV	23580	24423	1.96%	0.233%
47	13.739	1979	1981	1983	rBV2	20442	18821	1.51%	0.180%
48	13.804	1988	1992	1996	rVB4	44783	61131	4.91%	0.583%
49	13.986	2018	2023	2026	rBV2	966444	1014273	81.53%	9.681%
50	14.010	2026	2027	2036	rVB	124199	124126	9.98%	1.185%
51	15.033	2198	2201	2203	rBV	92163	113508	9.12%	1.083%
52	15.333	2250	2252	2255	rBV	53378	51552	4.14%	0.492%
53	15.398	2261	2263	2269	rBV2	64530	110408	8.87%	1.054%
54	15.462	2269	2274	2285	rVB	630761	862994	69.37%	8.237%


Sum of corrected areas: 10477331

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101535.D
Acq On : 19 Dec 2017 21:03
Operator : SJ/JU
Sample : I6981-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PHMHA-WCS

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

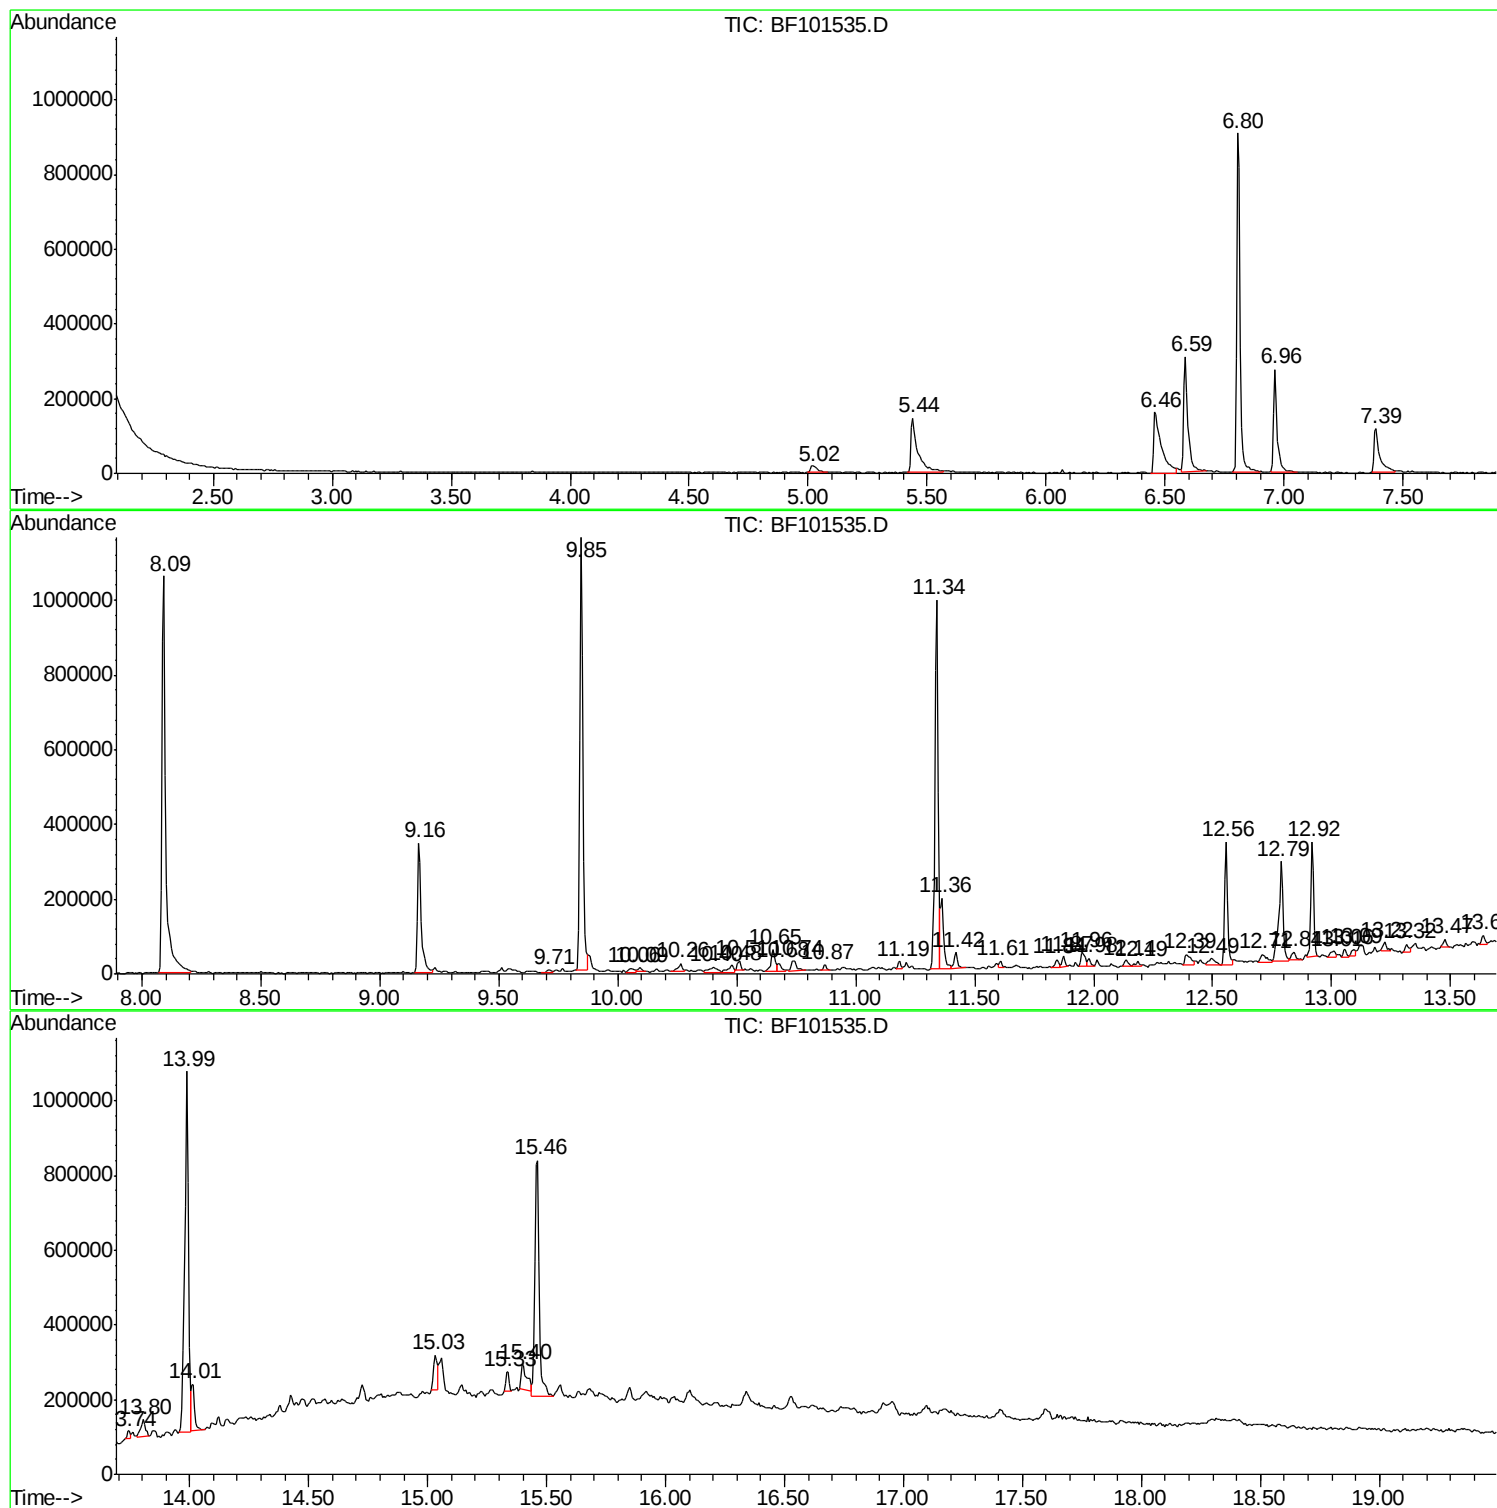

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101535.D
Acq On : 19 Dec 2017 21:03
Operator : SJ/JU
Sample : I6981-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PHMHA-WCS










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.59 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.59	8.10 ng	379223	1,4-Dichlorobenzene-d4	6.80

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
4		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

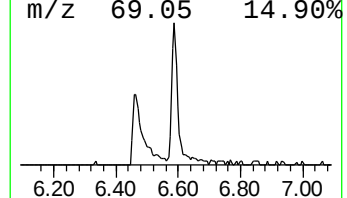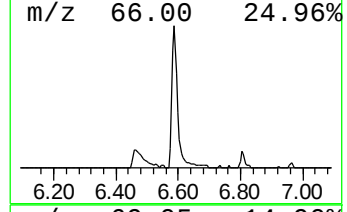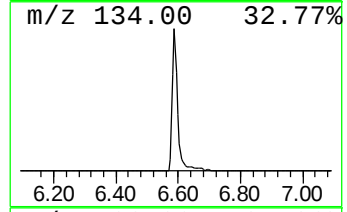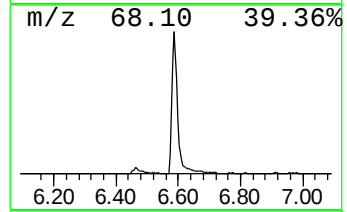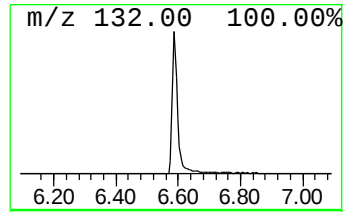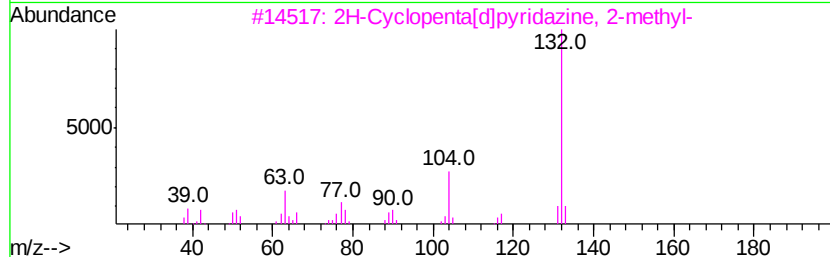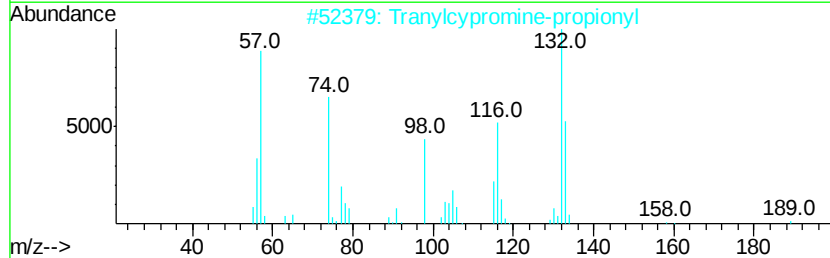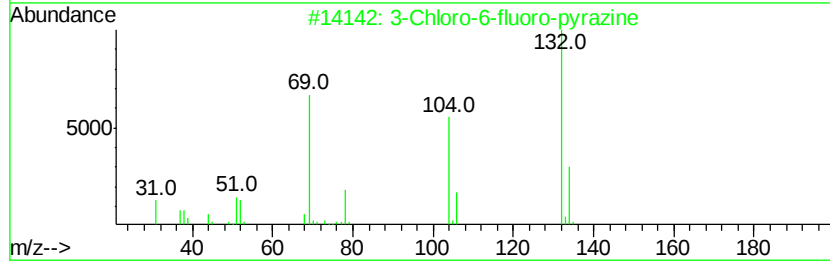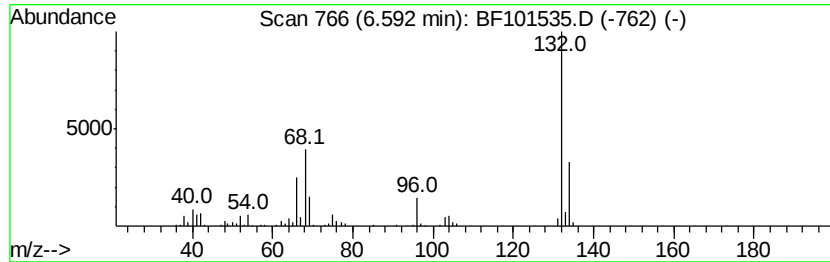

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121917\
Data File : BF101535.D
Acq On : 19 Dec 2017 21:03
Operator : SJ/JU
Sample : I6981-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PHMHA-WCS

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.59	6.59	8.1	ng	379223	1	6.80	936459	20.0