

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
 Data File : BF101550.D
 Acq On : 20 Dec 2017 4:57
 Operator : SJ/JU
 Sample : I6956-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 121417--DBRI-E-U-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	496	500	508	rBV	36206	70712	1.81%	0.293%
2	5.428	565	568	601	rBV	796831	1257982	32.14%	5.206%
3	6.451	739	742	760	rBV	478465	816152	20.85%	3.377%
4	6.581	760	764	771	rBV	1974296	2134032	54.53%	8.831%
5	6.804	799	802	811	rBV	1002088	951762	24.32%	3.939%
6	6.963	825	829	845	rBV	2900836	2834438	72.43%	11.730%
7	7.375	895	899	924	rBV	2132519	2535526	64.79%	10.493%
8	8.092	1017	1021	1045	rBV	1055034	1266930	32.37%	5.243%
9	9.163	1199	1203	1213	rBV	3927004	3913598	100.00%	16.195%
10	9.569	1266	1272	1277	rBV	43176	52279	1.34%	0.216%
11	9.845	1309	1319	1333	rBV	1246973	1304851	33.34%	5.400%
12	10.257	1387	1389	1393	rVB	54782	42499	1.09%	0.176%
13	10.639	1450	1454	1467	rBV	1201867	1395491	35.66%	5.775%
14	11.339	1569	1573	1589	rBV	949032	1083834	27.69%	4.485%
15	12.915	1837	1841	1845	rBV	2582640	2619980	66.95%	10.842%
16	13.804	1988	1992	2002	rBV5	28545	58360	1.49%	0.242%
17	13.986	2019	2023	2034	rBV	783841	861531	22.01%	3.565%
18	14.580	2121	2124	2128	rBV	45426	48636	1.24%	0.201%
19	15.456	2269	2273	2283	rVB	576743	866996	22.15%	3.588%
20	16.333	2418	2422	2427	rBV3	28485	49202	1.26%	0.204%


Sum of corrected areas: 24164791

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101550.D
Acq On : 20 Dec 2017 4:57
Operator : SJ/JU
Sample : I6956-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121417--DBRI-E-U-M

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

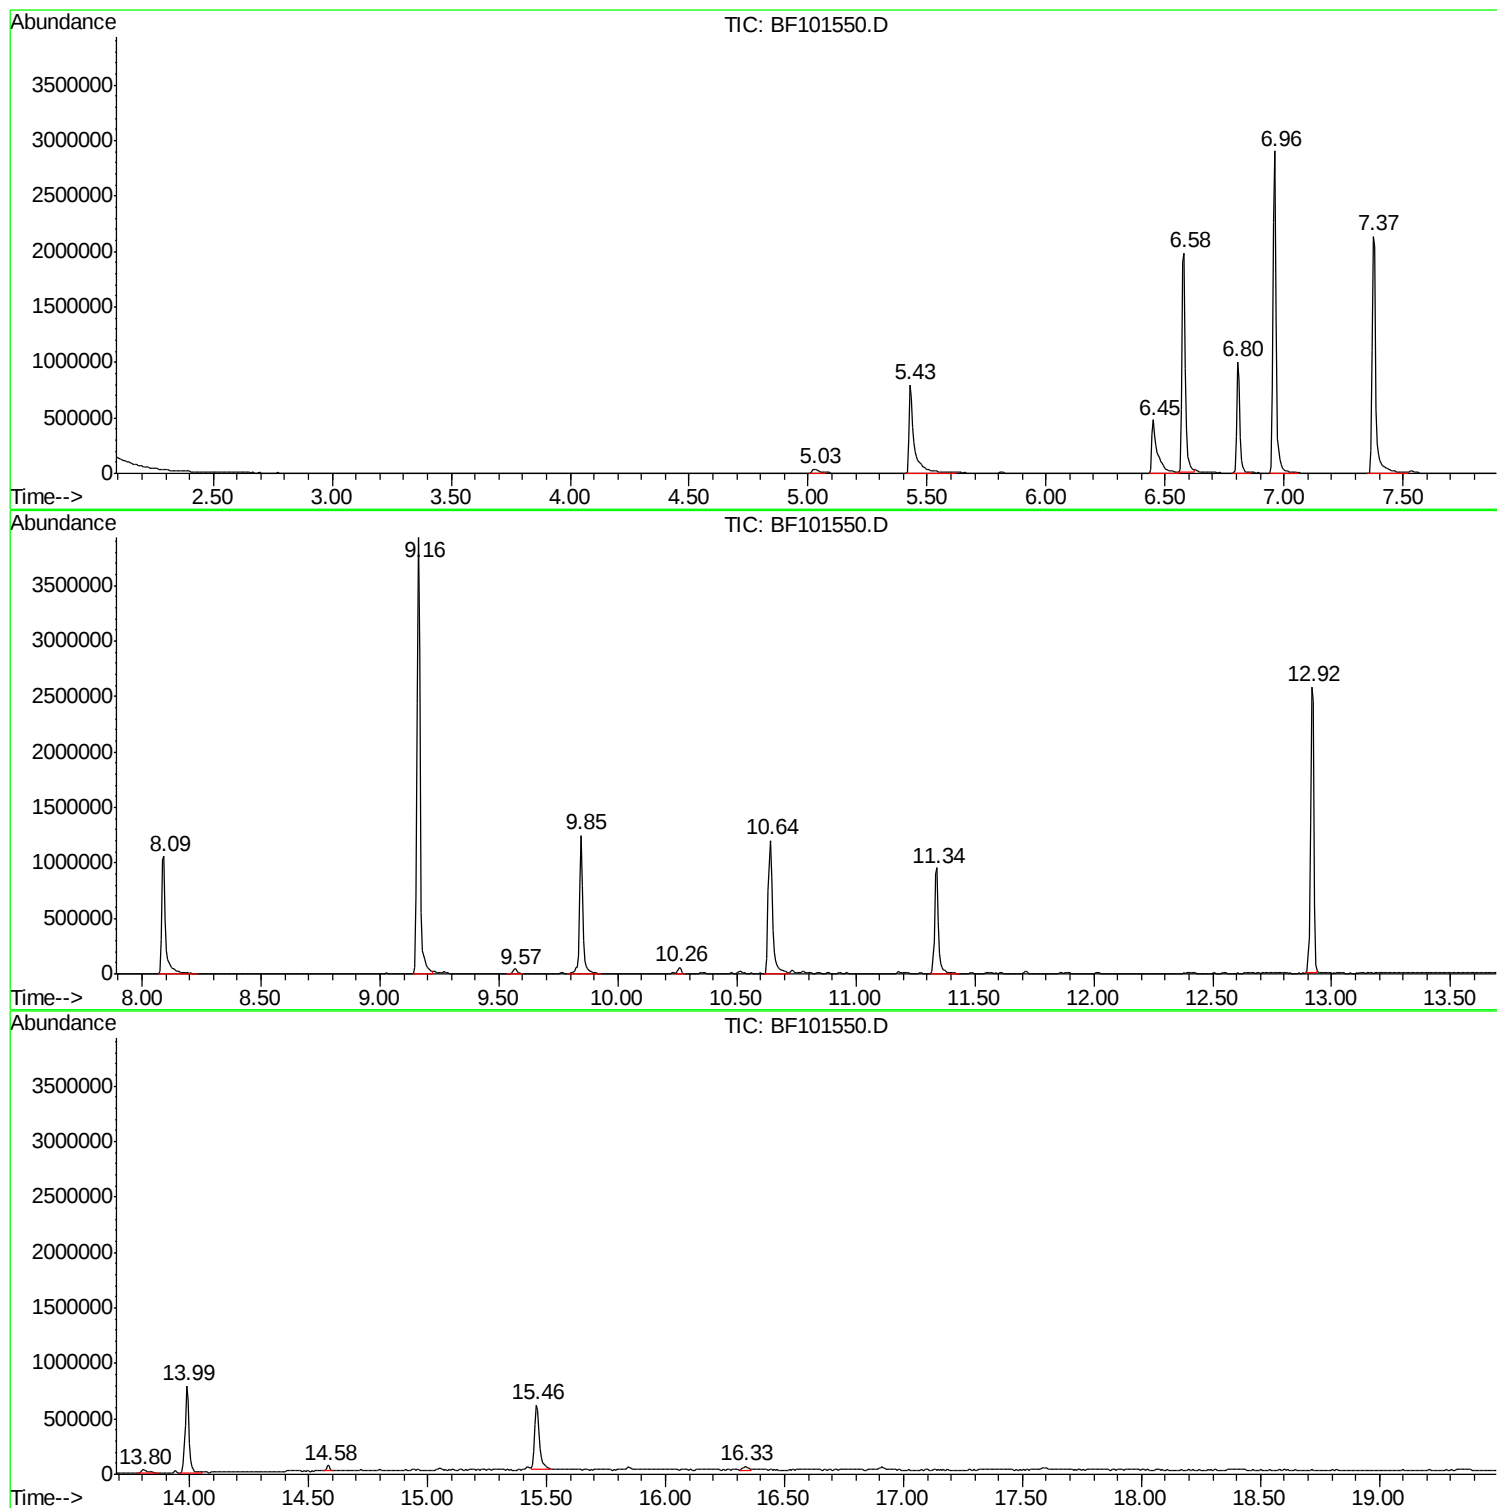

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101550.D
Acq On : 20 Dec 2017 4:57
Operator : SJ/JU
Sample : I6956-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121417-DBRI-E-U-M










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.58 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.58	44.84 ng	2134030	1,4-Dichlorobenzene-d4	6.80

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine			132	C4H2ClFN2	1000146-10-7	27
2	5-Aminoindole			132	C8H8N2	005192-03-0	12
3	Tranvlcvpromine-propionyl			189	C12H15NO	1000123-86-3	10
4	Bicyclo[4.2.0]octa-1,3,5-triene,...			132	C10H12	028749-81-7	9
5	4-Chloro-2-fluoro-pyrimidine			132	C4H2ClFN2	051422-00-5	9

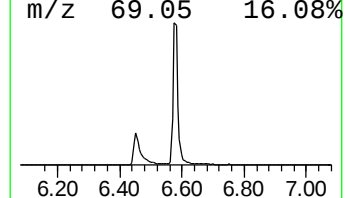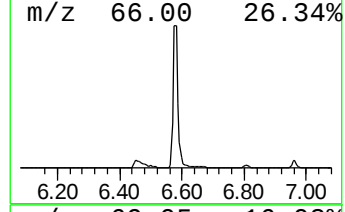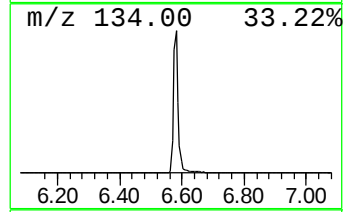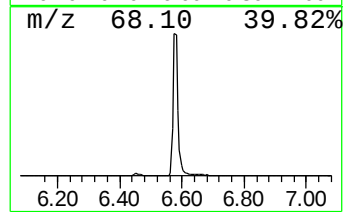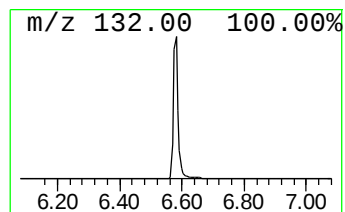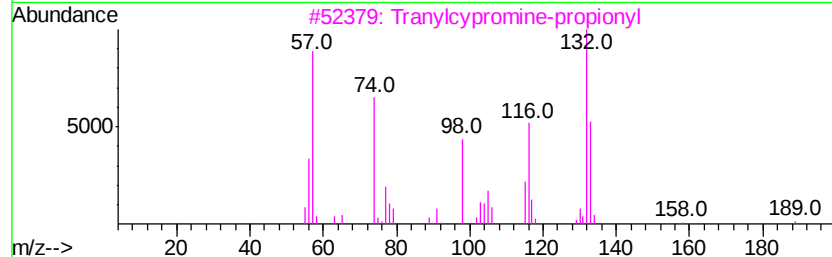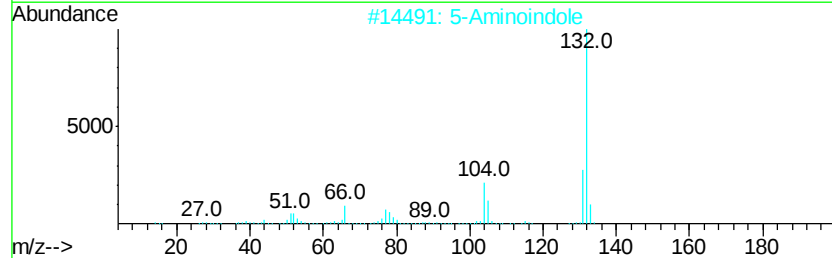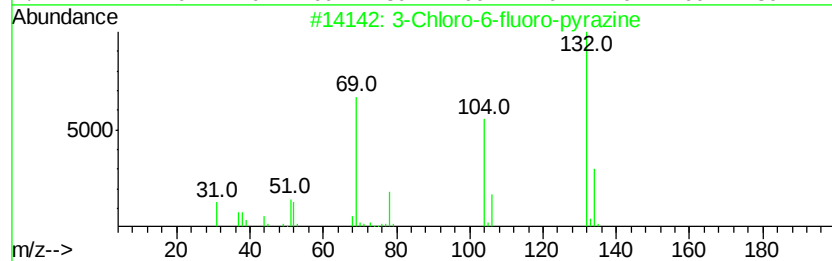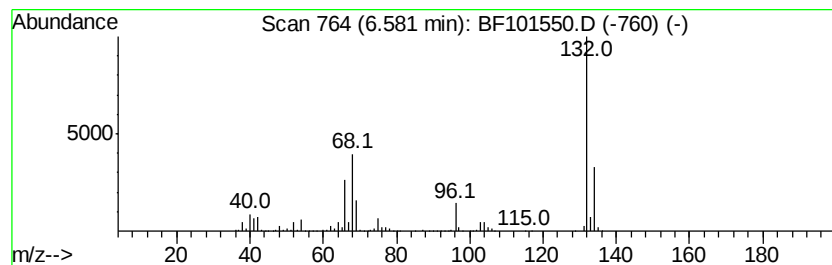

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121917\
Data File : BF101550.D
Acq On : 20 Dec 2017 4:57
Operator : SJ/JU
Sample : I6956-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121417--DBRI-E-U-M

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.58	6.58	44.8	ng	2134030	1	6.80	951762	20.0