

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121917\
 Data File : BF101551.D
 Acq On : 20 Dec 2017 5:24
 Operator : SJ/JU
 Sample : I6956-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 121417-TIDO-E-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	497	500	515	rBV	36074	77451	1.75%	0.282%
2	5.428	565	568	592	rBV	949650	1421199	32.18%	5.177%
3	6.451	738	742	760	rBV	560557	965838	21.87%	3.518%
4	6.581	760	764	771	rBV	2282675	2436119	55.16%	8.874%
5	6.804	799	802	811	rBV	1049640	999702	22.64%	3.641%
6	6.963	825	829	845	rBV	3178936	3154280	71.42%	11.490%
7	7.381	895	900	922	rBV	2457322	2878389	65.17%	10.485%
8	8.086	1017	1020	1038	rBV	1150032	1342061	30.39%	4.888%
9	9.163	1199	1203	1213	rBV	4144923	4416445	100.00%	16.087%
10	9.563	1268	1271	1278	rVB	81801	91666	2.08%	0.334%
11	9.845	1312	1319	1323	rBV	1367925	1391724	31.51%	5.069%
12	9.875	1323	1324	1333	rVB	110488	99964	2.26%	0.364%
13	10.257	1386	1389	1396	rVB	206415	170606	3.86%	0.621%
14	10.639	1450	1454	1467	rBV	1563399	1723482	39.02%	6.278%
15	11.339	1569	1573	1581	rBV	1102283	1199800	27.17%	4.370%
16	11.551	1603	1609	1614	rBV3	52435	83423	1.89%	0.304%
17	12.369	1744	1748	1752	rBV	45288	70257	1.59%	0.256%
18	12.416	1752	1756	1759	rVB2	82711	78803	1.78%	0.287%
19	12.563	1775	1781	1787	rBV	55009	64501	1.46%	0.235%
20	12.921	1837	1842	1845	rBV	3023939	2999401	67.91%	10.925%
21	13.804	1989	1992	2003	rBV6	22940	44246	1.00%	0.161%
22	13.986	2019	2023	2032	rBV	801785	868239	19.66%	3.163%
23	15.457	2268	2273	2286	rVB	555719	875986	19.83%	3.191%


Sum of corrected areas: 27453582

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101551.D
Acq On : 20 Dec 2017 5:24
Operator : SJ/JU
Sample : I6956-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121417-TIDO-E-D-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

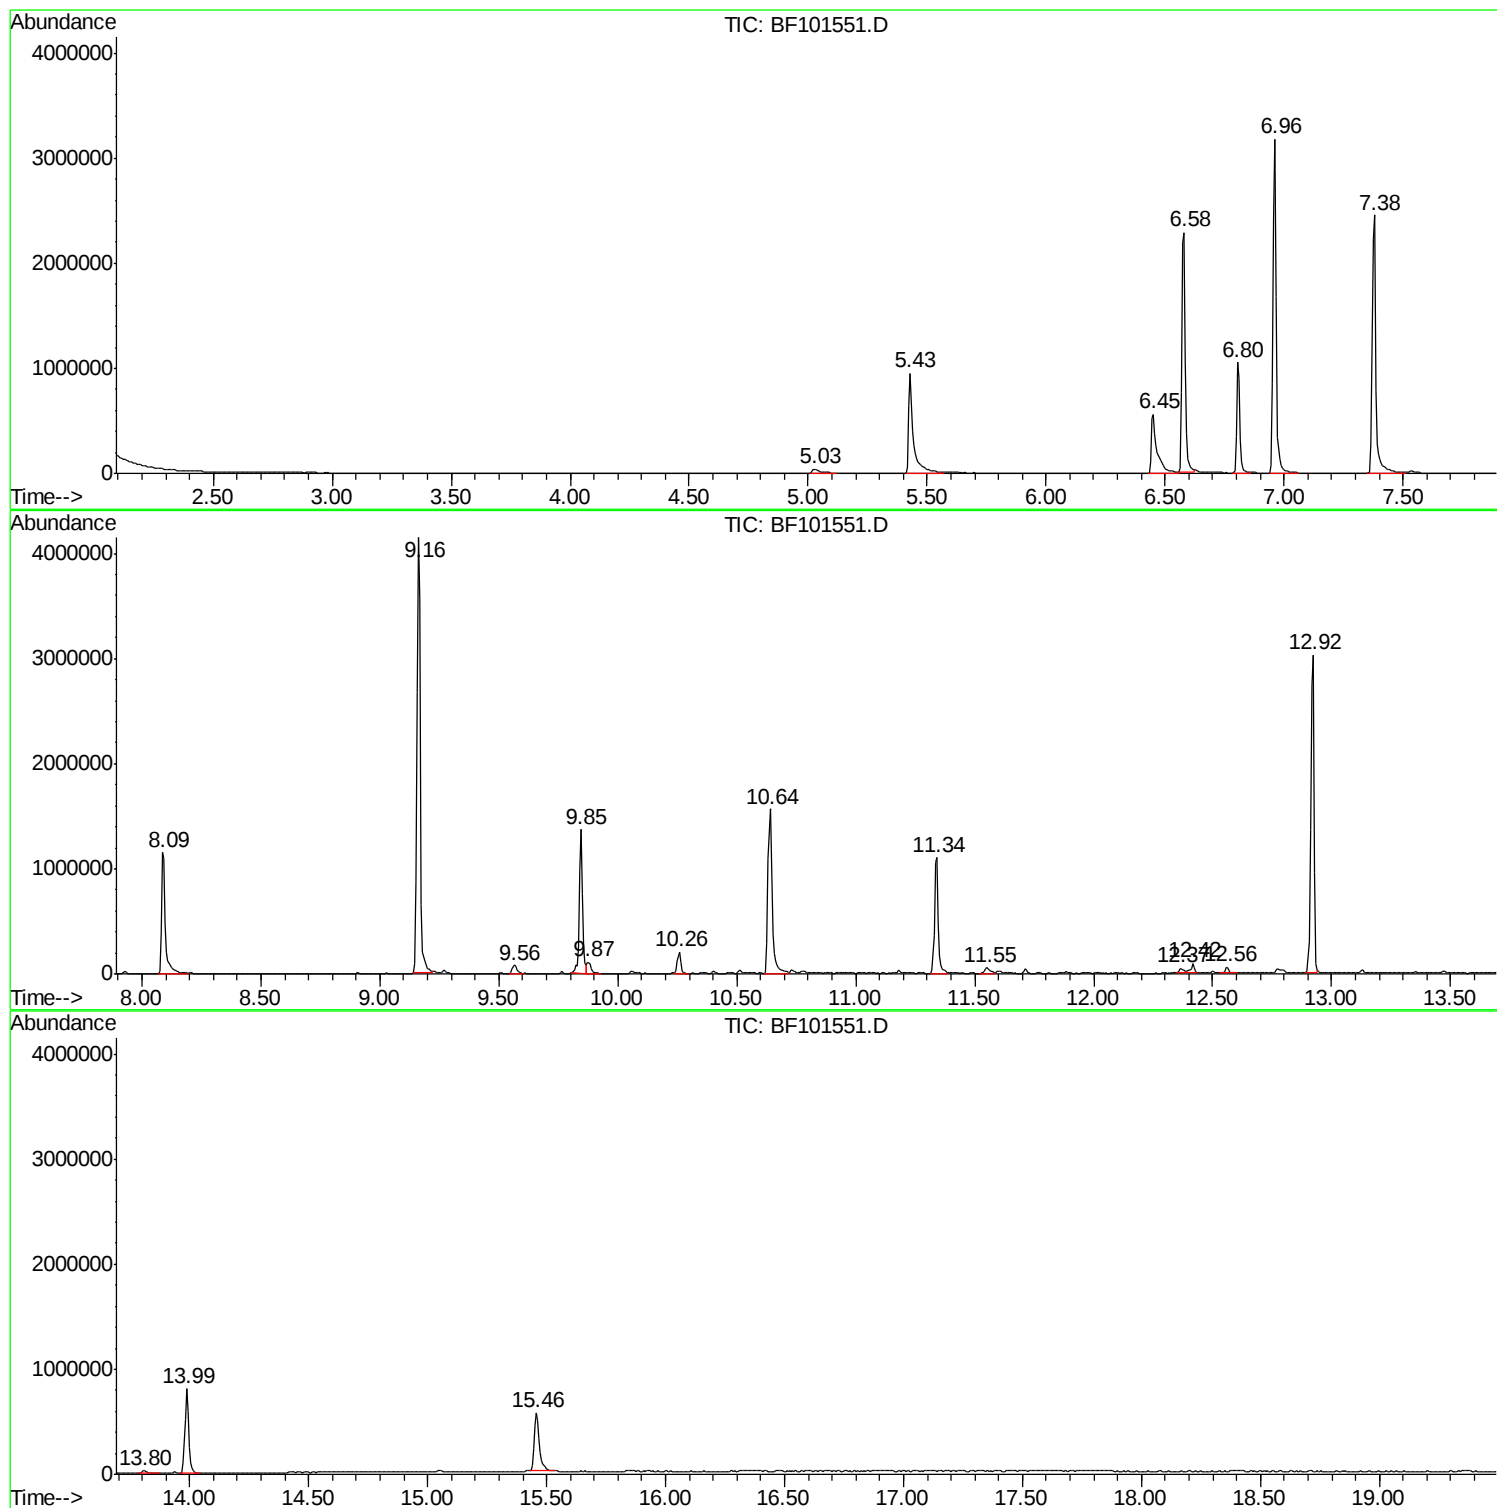

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101551.D
Acq On : 20 Dec 2017 5:24
Operator : SJ/JU
Sample : I6956-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121417-TIDO-E-D-B










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.58 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.58	48.74 ng	2436120	1,4-Dichlorobenzene-d4	6.80

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

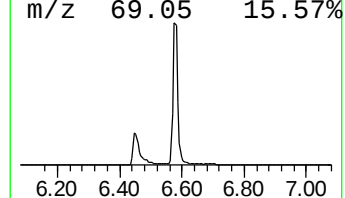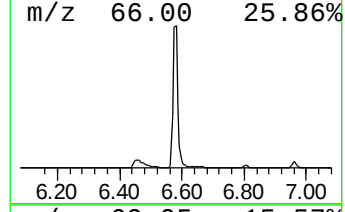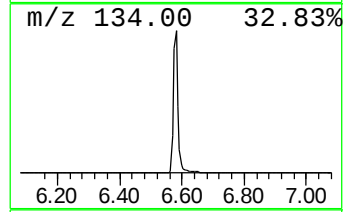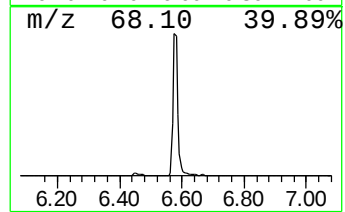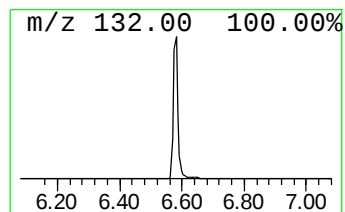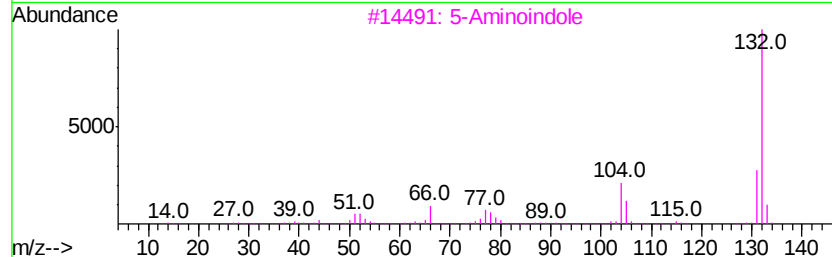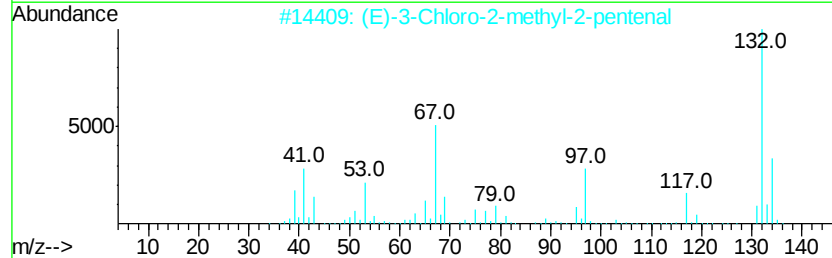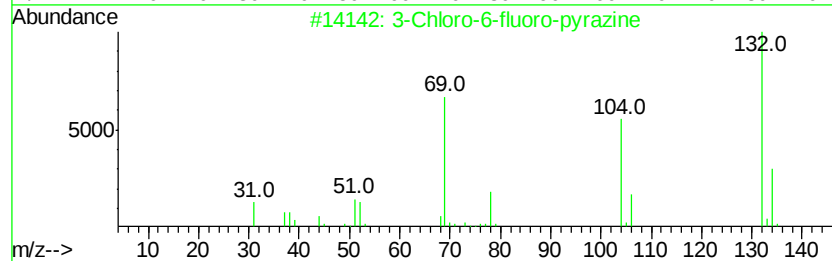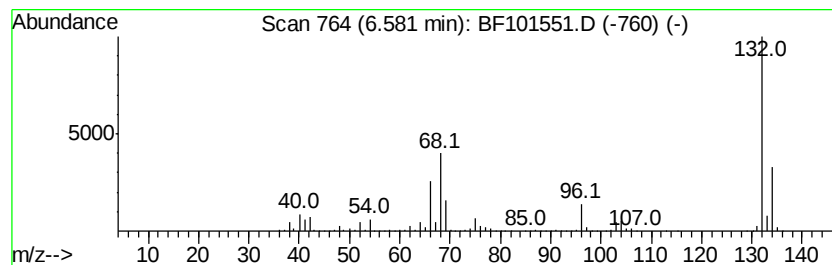

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121917\
Data File : BF101551.D
Acq On : 20 Dec 2017 5:24
Operator : SJ/JU
Sample : I6956-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121417-TIDO-E-D-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.58	6.58	48.7	ng	2436120	1	6.80	999702	20.0