

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
 Data File : BF101553.D
 Acq On : 20 Dec 2017 6:18
 Operator : SJ/JU
 Sample : I6956-05
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 121417-TIDO-E-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	496	500	517	rBV	34926	76475	1.87%	0.303%
2	5.428	565	568	586	rBV	881089	1263934	30.93%	5.004%
3	6.451	739	742	760	rBV	509608	881217	21.56%	3.489%
4	6.581	760	764	778	rVB	2086437	2288330	55.99%	9.060%
5	6.804	799	802	812	rBV	1002960	973857	23.83%	3.856%
6	6.963	825	829	847	rBV	3023071	2970809	72.69%	11.763%
7	7.380	895	900	924	rBV	2237566	2667053	65.26%	10.560%
8	8.092	1017	1021	1038	rBV	1075039	1278392	31.28%	5.062%
9	9.163	1199	1203	1214	rBV	4044113	4086979	100.00%	16.182%
10	9.563	1265	1271	1278	rBV	84617	101357	2.48%	0.401%
11	9.845	1313	1319	1332	rVB	1255670	1319990	32.30%	5.226%
12	10.639	1450	1454	1468	rBV	1305942	1548565	37.89%	6.131%
13	11.339	1569	1573	1587	rBV	1008382	1165102	28.51%	4.613%
14	12.921	1837	1842	1845	rBV	2694612	2776744	67.94%	10.994%
15	13.804	1988	1992	2006	rBV2	70602	134931	3.30%	0.534%
16	13.986	2019	2023	2033	rBV	839465	861774	21.09%	3.412%
17	15.456	2268	2273	2284	rVB	595471	861015	21.07%	3.409%


Sum of corrected areas: 25256524

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101553.D
Acq On : 20 Dec 2017 6:18
Operator : SJ/JU
Sample : I6956-05
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121417-TIDO-E-U-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

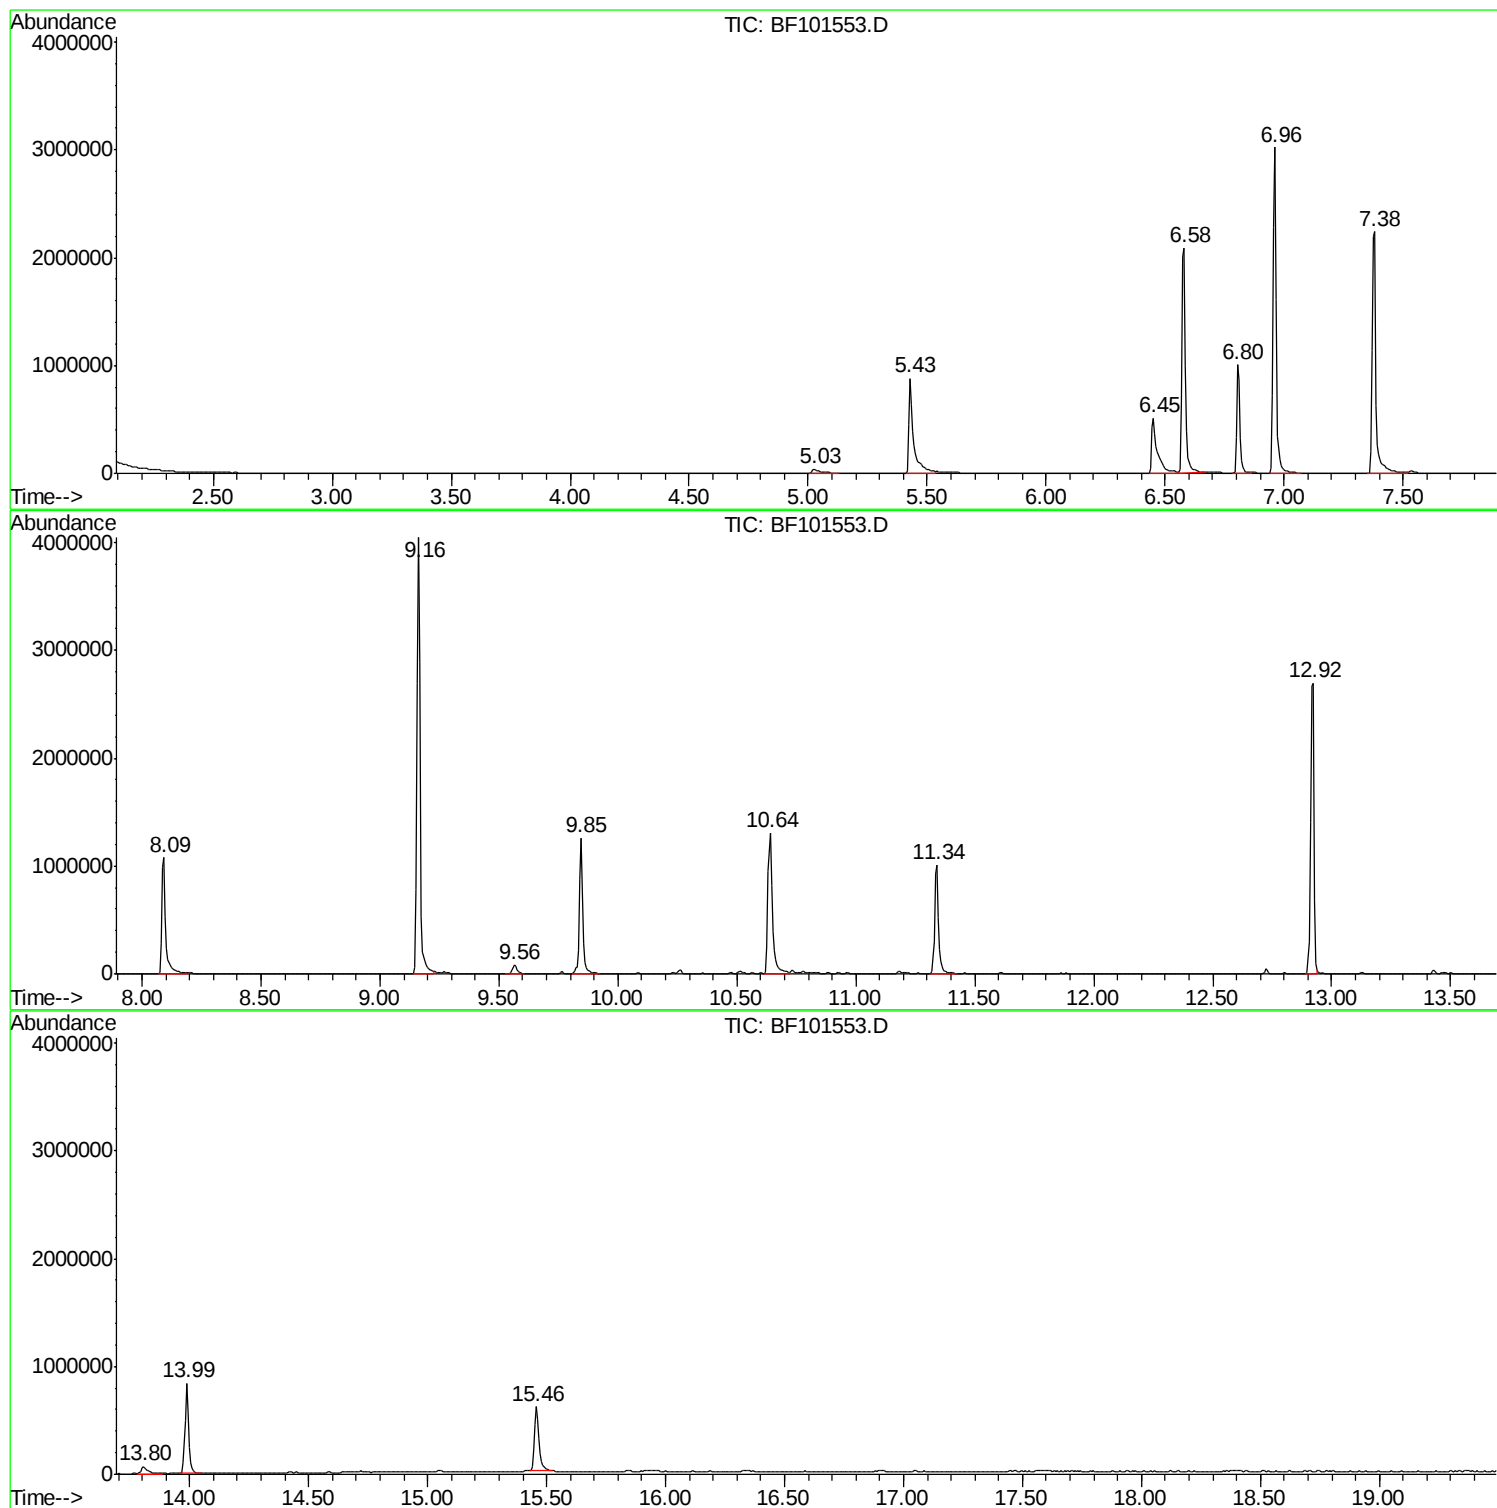

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101553.D
Acq On : 20 Dec 2017 6:18
Operator : SJ/JU
Sample : I6956-05
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121417-TIDO-E-U-B










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.58 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.58	47.00 ng	2288330	1,4-Dichlorobenzene-d4	6.80

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine			132	C4H2ClFN2	1000146-10-7	27
2	5-Aminoindole			132	C8H8N2	005192-03-0	12
3	Tranvlcvpromine-propionyl			189	C12H15NO	1000123-86-3	10
4	Imidazole, 4,5-dicvano-1-methyl-			132	C6H4N4	019485-35-9	9
5	1,3,5-Trifluorobenzene			132	C6H3F3	000372-38-3	9

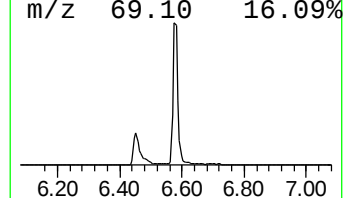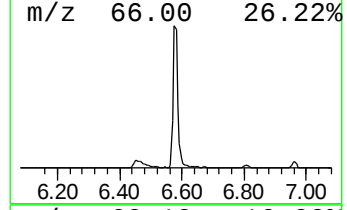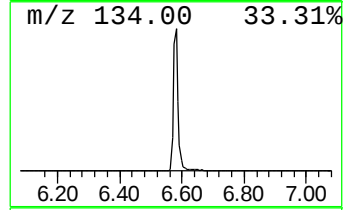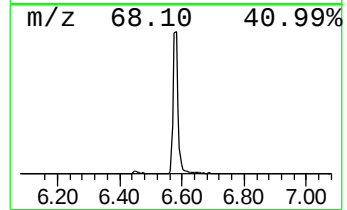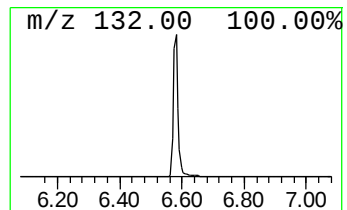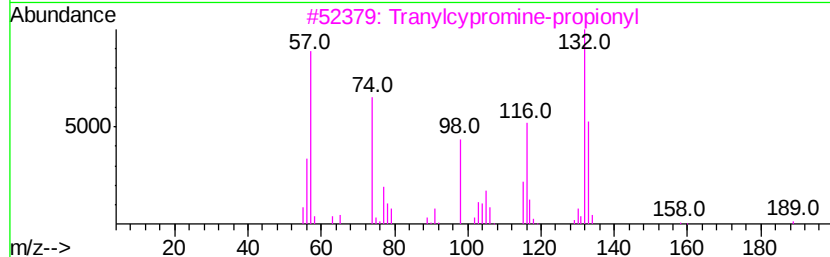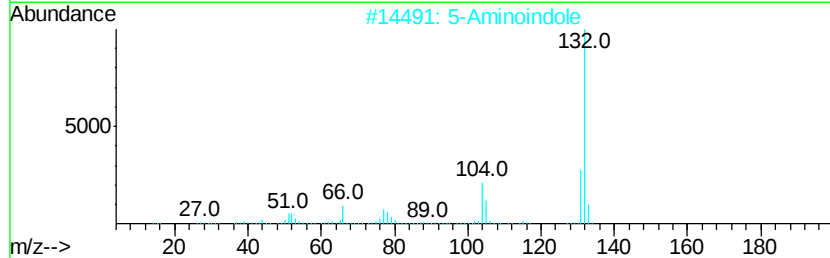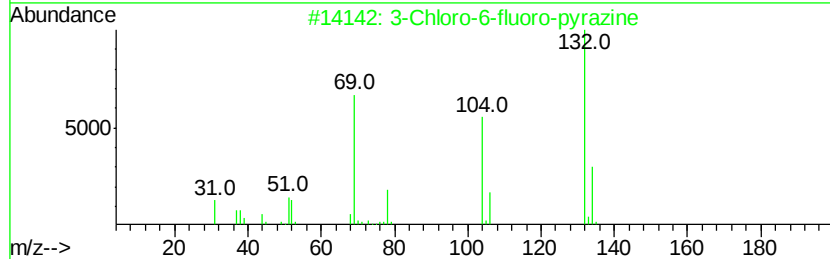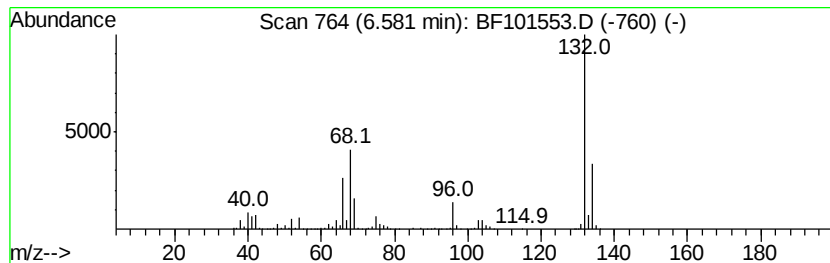

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101553.D
Acq On : 20 Dec 2017 6:18
Operator : SJ/JU
Sample : I6956-05
Misc :
ALS Vial : 36 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
121417-TIDO-E-U-B

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Dichloroacetic acid, heptad... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.		
13.80	3.13 ng	134931	Chrysene-d12	13.99		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	95
2		Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	93
3		Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	93
4		Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	91
5		17-Pentatriacontene	491	C35H70	006971-40-0	91

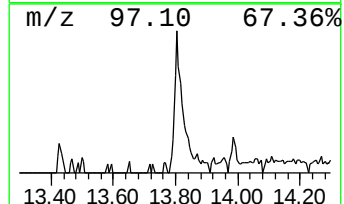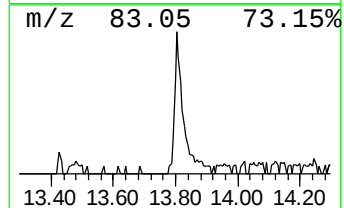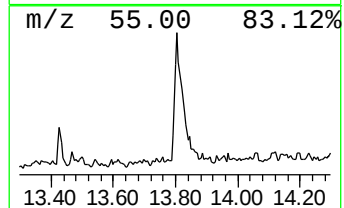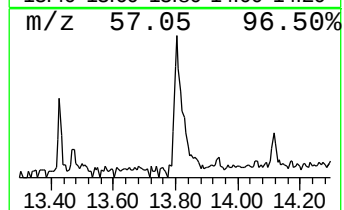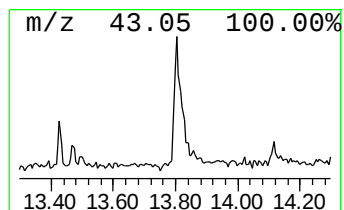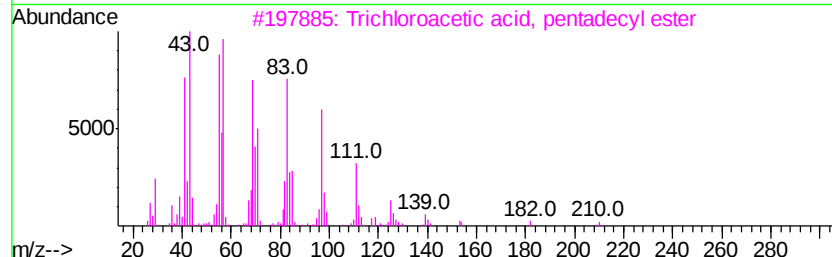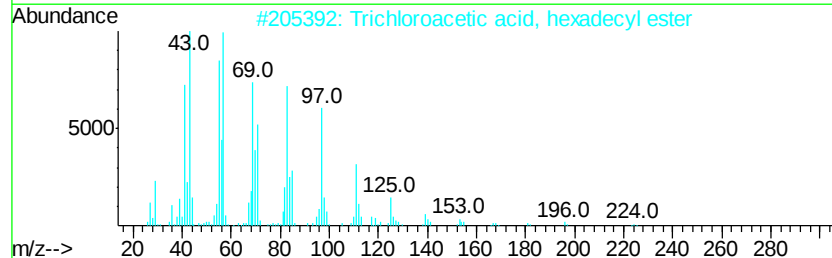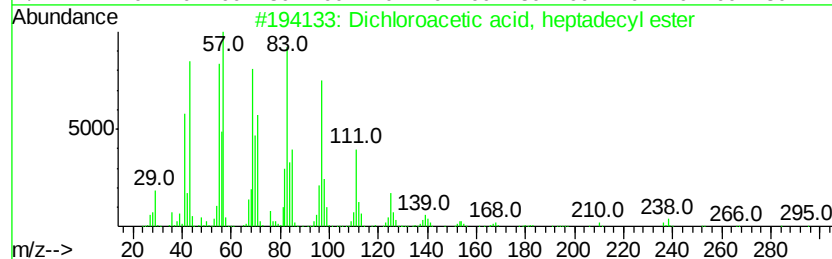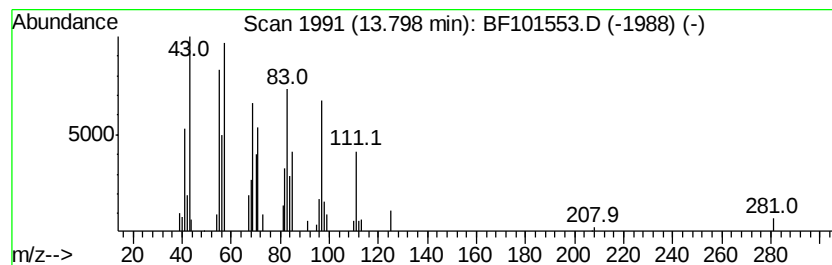

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121917\
Data File : BF101553.D
Acq On : 20 Dec 2017 6:18
Operator : SJ/JU
Sample : I6956-05
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121417-TIDO-E-U-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.58	6.58	47.0	ng	2288330	1	6.80	973857	20.0
Dichloroacetic ac...	13.80	3.1	ng	134931	5	13.99	861774	20.0