

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
 Data File : BF101555.D
 Acq On : 20 Dec 2017 7:11
 Operator : SJ/JU
 Sample : I6956-07
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 121417-JETT-E-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	497	500	515	rBV	27519	58747	1.38%	0.225%
2	5.428	565	568	596	rBV	864184	1345754	31.62%	5.143%
3	6.451	739	742	760	rBV	503359	860319	20.21%	3.288%
4	6.575	760	763	779	rVB	2145840	2371167	55.71%	9.063%
5	6.804	799	802	812	rBV	998425	973174	22.87%	3.719%
6	6.963	825	829	846	rBV	3017142	2994081	70.35%	11.443%
7	7.375	895	899	924	rBV	2238442	2732504	64.20%	10.444%
8	8.086	1017	1020	1039	rBV	1079418	1286755	30.23%	4.918%
9	9.163	1199	1203	1214	rBV	4092449	4255911	100.00%	16.266%
10	9.563	1268	1271	1278	rVB	85494	95019	2.23%	0.363%
11	9.845	1312	1319	1333	rBV	1322496	1365052	32.07%	5.217%
12	10.639	1450	1454	1467	rBV	1456550	1710403	40.19%	6.537%
13	11.333	1569	1572	1590	rVB	1034028	1226129	28.81%	4.686%
14	12.921	1837	1842	1845	rBV	2914975	3012407	70.78%	11.513%
15	13.804	1988	1992	2008	rBV2	69697	141534	3.33%	0.541%
16	13.986	2019	2023	2033	rBV	822209	864245	20.31%	3.303%
17	15.456	2268	2273	2288	rVB2	555978	871120	20.47%	3.329%


Sum of corrected areas: 26164321

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101555.D
Acq On : 20 Dec 2017 7:11
Operator : SJ/JU
Sample : I6956-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121417-JETT-E-D-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

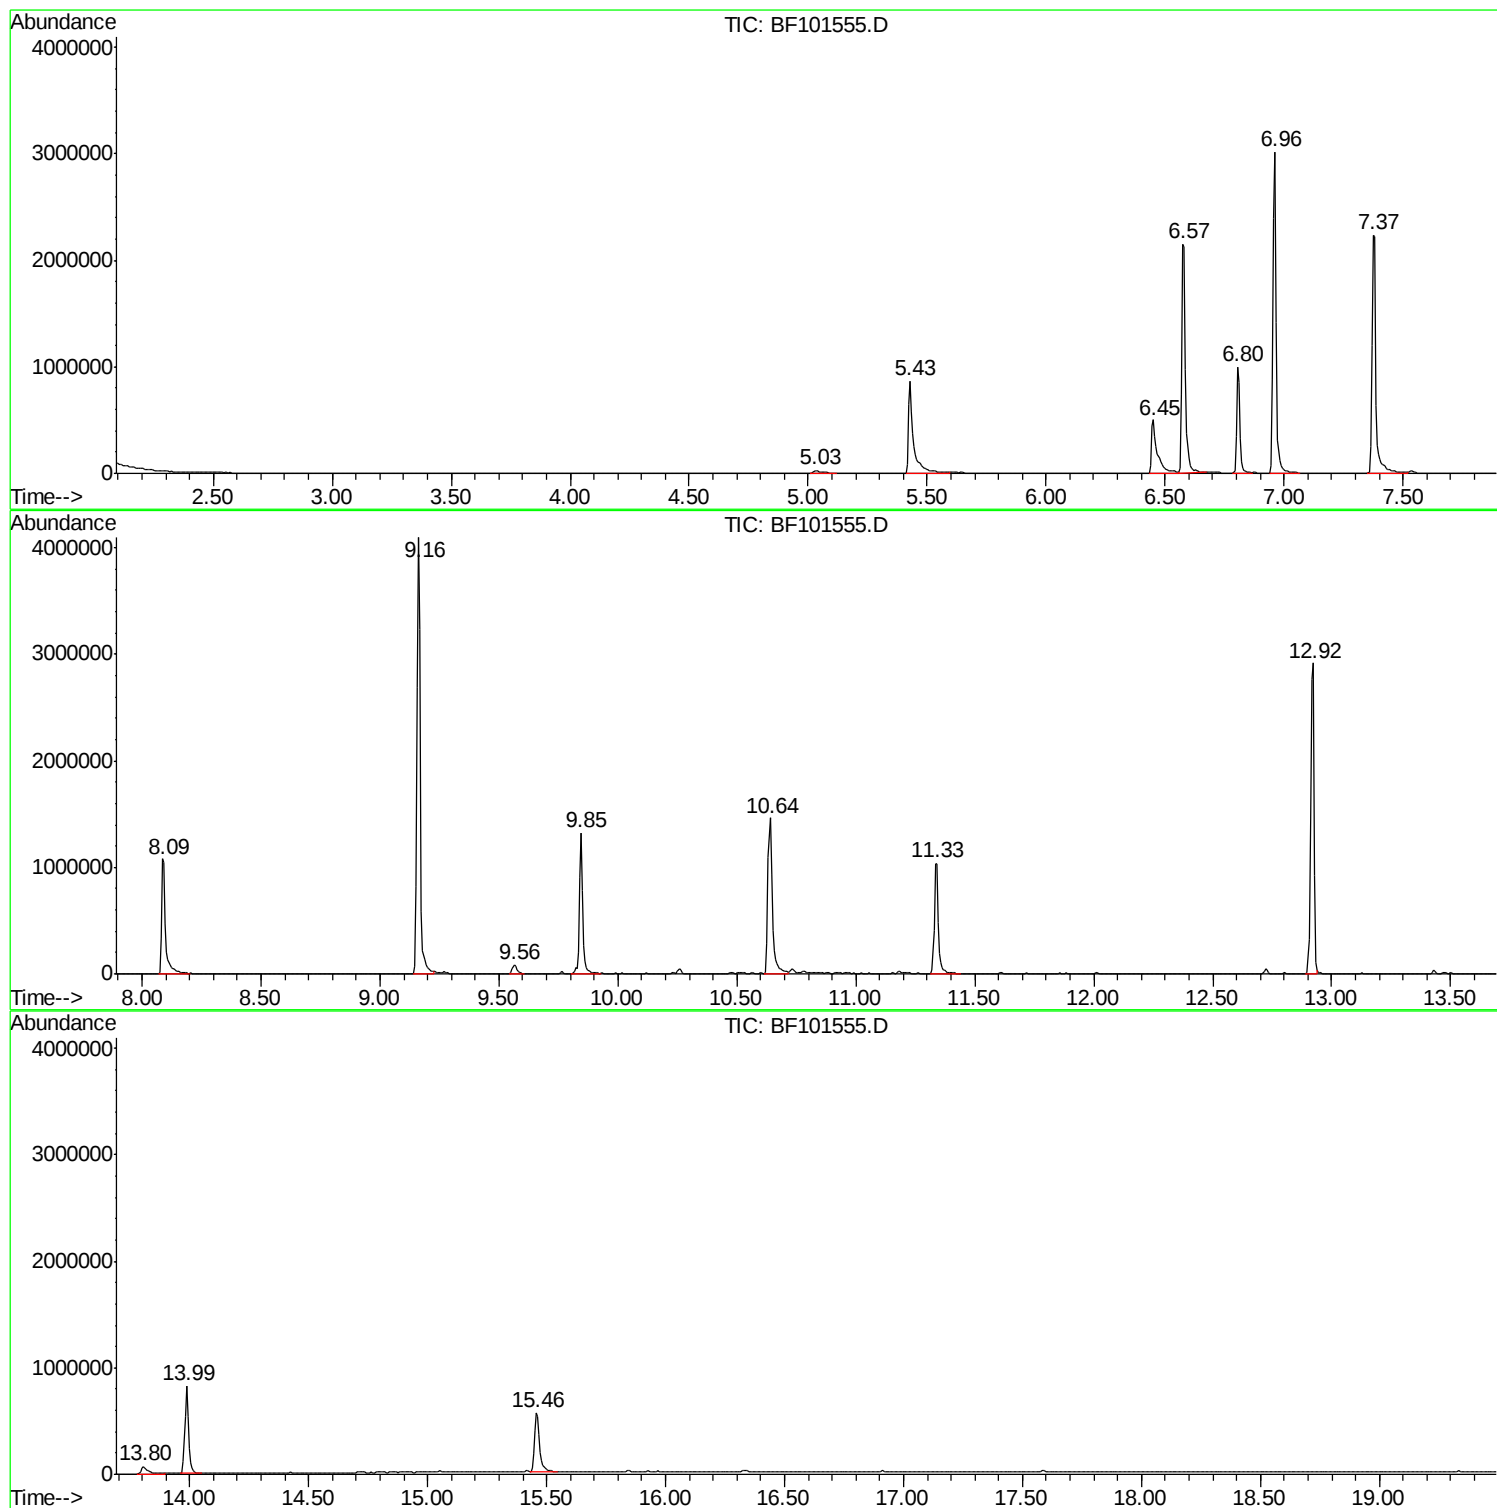

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101555.D
Acq On : 20 Dec 2017 7:11
Operator : SJ/JU
Sample : I6956-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121417-JETT-E-D-B










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.57 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.57	48.73 ng	2371170	1,4-Dichlorobenzene-d4	6.80

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9

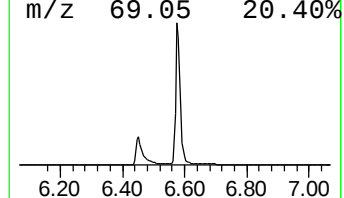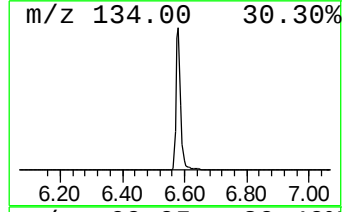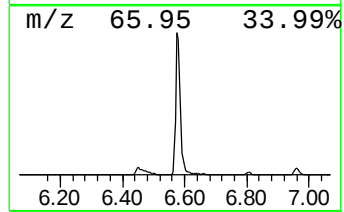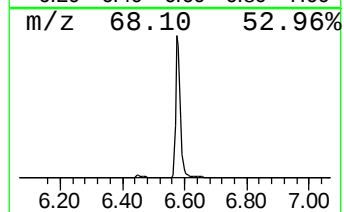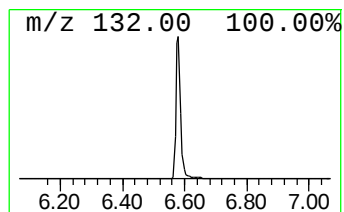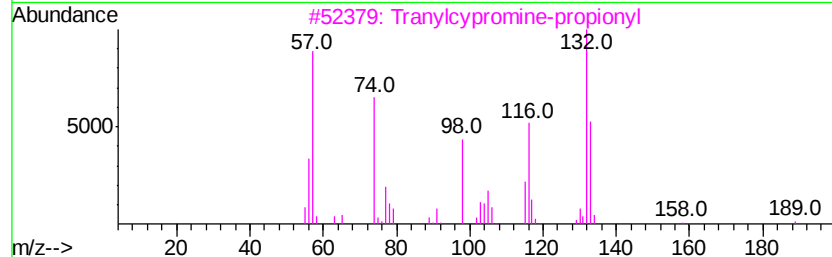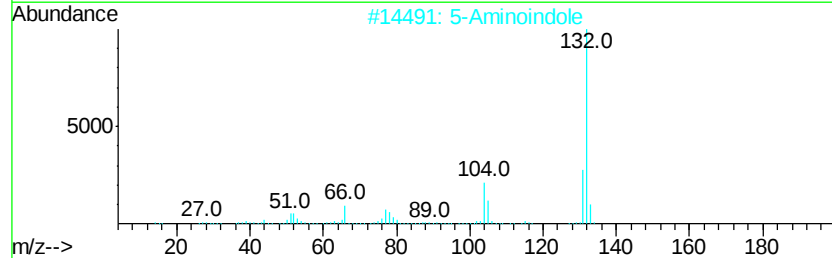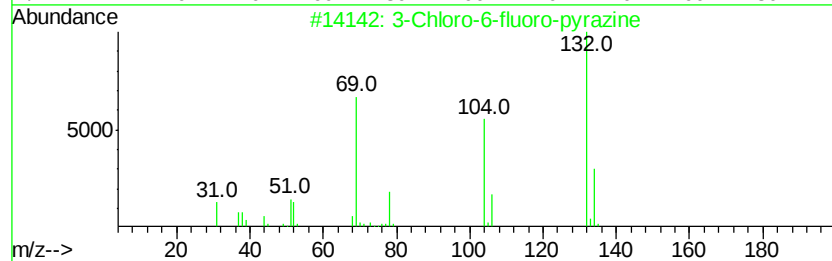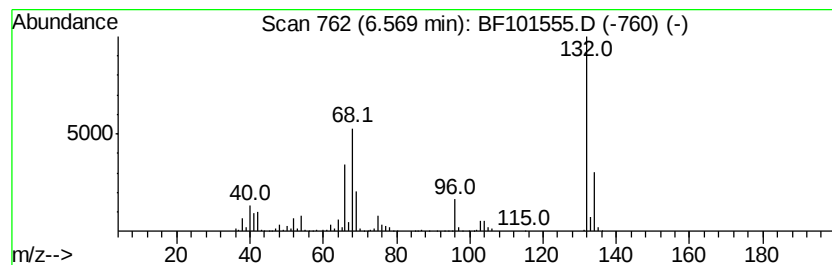

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101555.D
Acq On : 20 Dec 2017 7:11
Operator : SJ/JU
Sample : I6956-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121417-JETT-E-D-B










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Trifluoroacetoxy hexadecane Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.80	3.28 ng	141534	Chrysene-d12	13.99

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	90
2		17-Pentatriacontene	491	C35H70	006971-40-0	87
3		5-Eicosene, (E)-	280	C20H40	074685-30-6	86
4		1-Octadecanol	270	C18H38O	000112-92-5	83
5		Octadecyl trifluoroacetate	366	C20H37F3O2	079392-43-1	80

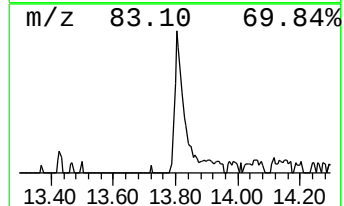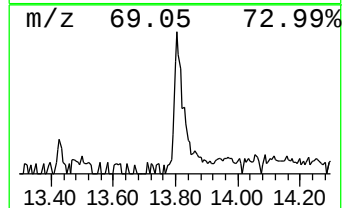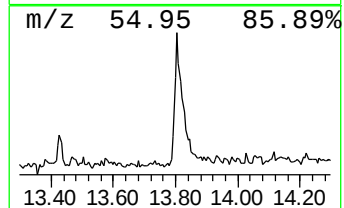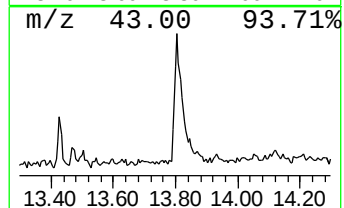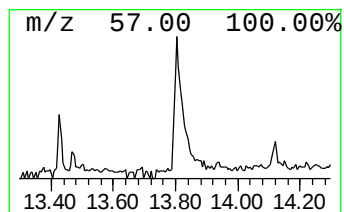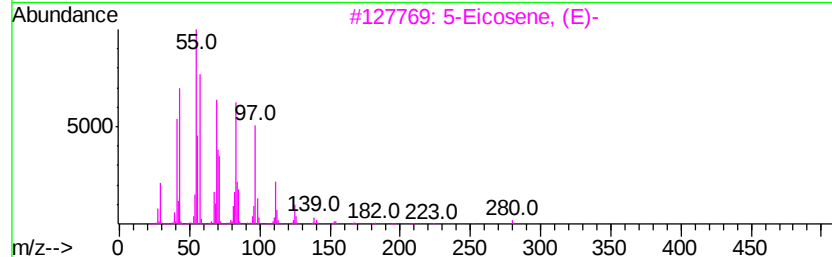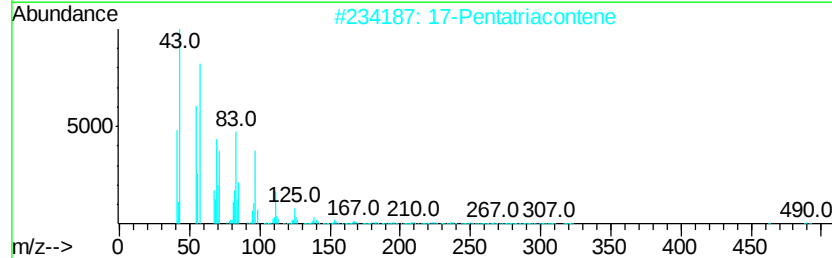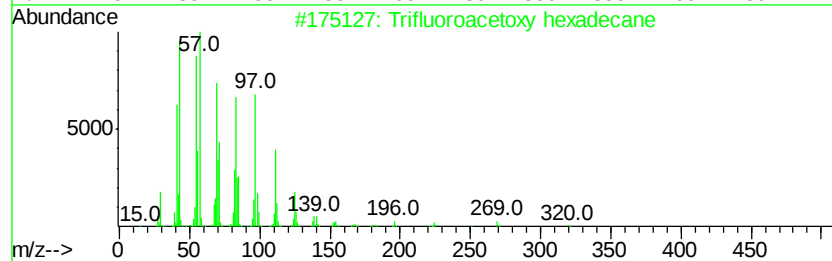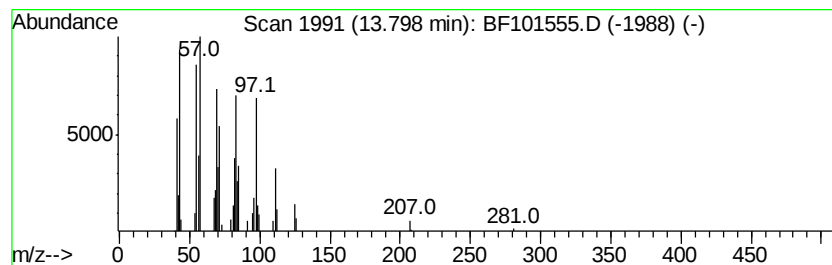

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121917\
Data File : BF101555.D
Acq On : 20 Dec 2017 7:11
Operator : SJ/JU
Sample : I6956-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121417-JETT-E-D-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.57	6.57	48.7	ng	2371170	1	6.80	973174	20.0
Trifluoroacetoxy ...	13.80	3.3	ng	141534	5	13.99	864245	20.0