

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
 Data File : BF101556.D
 Acq On : 20 Dec 2017 7:38
 Operator : SJ/JU
 Sample : I6956-08
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 121417-JETT-E-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	496	500	517	rBV	33247	71700	1.77%	0.289%
2	5.428	565	568	598	rBV	782531	1238463	30.51%	4.998%
3	6.451	738	742	756	rBV	487104	825350	20.33%	3.331%
4	6.575	760	763	771	rBV	1908976	2103678	51.82%	8.490%
5	6.804	799	802	819	rVB	1048632	995850	24.53%	4.019%
6	6.963	825	829	849	rVB	2770623	2792161	68.78%	11.269%
7	7.375	895	899	924	rBV	2233602	2527265	62.25%	10.199%
8	8.086	1017	1020	1038	rBV	1111825	1304007	32.12%	5.263%
9	9.163	1199	1203	1219	rBV	3973560	4059736	100.00%	16.384%
10	9.569	1267	1272	1278	rBV	38355	51108	1.26%	0.206%
11	9.845	1312	1319	1332	rBV	1257948	1367630	33.69%	5.519%
12	10.639	1450	1454	1468	rBV	1277864	1531522	37.72%	6.181%
13	11.339	1569	1573	1587	rBV	1031101	1207300	29.74%	4.872%
14	12.921	1837	1842	1845	rBV	2789031	2892527	71.25%	11.674%
15	13.804	1988	1992	2007	rBV2	43802	106392	2.62%	0.429%
16	13.986	2019	2023	2034	rBV	805555	857227	21.12%	3.460%
17	15.457	2268	2273	2283	rVB	533770	846440	20.85%	3.416%


Sum of corrected areas: 24778356

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101556.D
Acq On : 20 Dec 2017 7:38
Operator : SJ/JU
Sample : I6956-08
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121417-JETT-E-D-S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

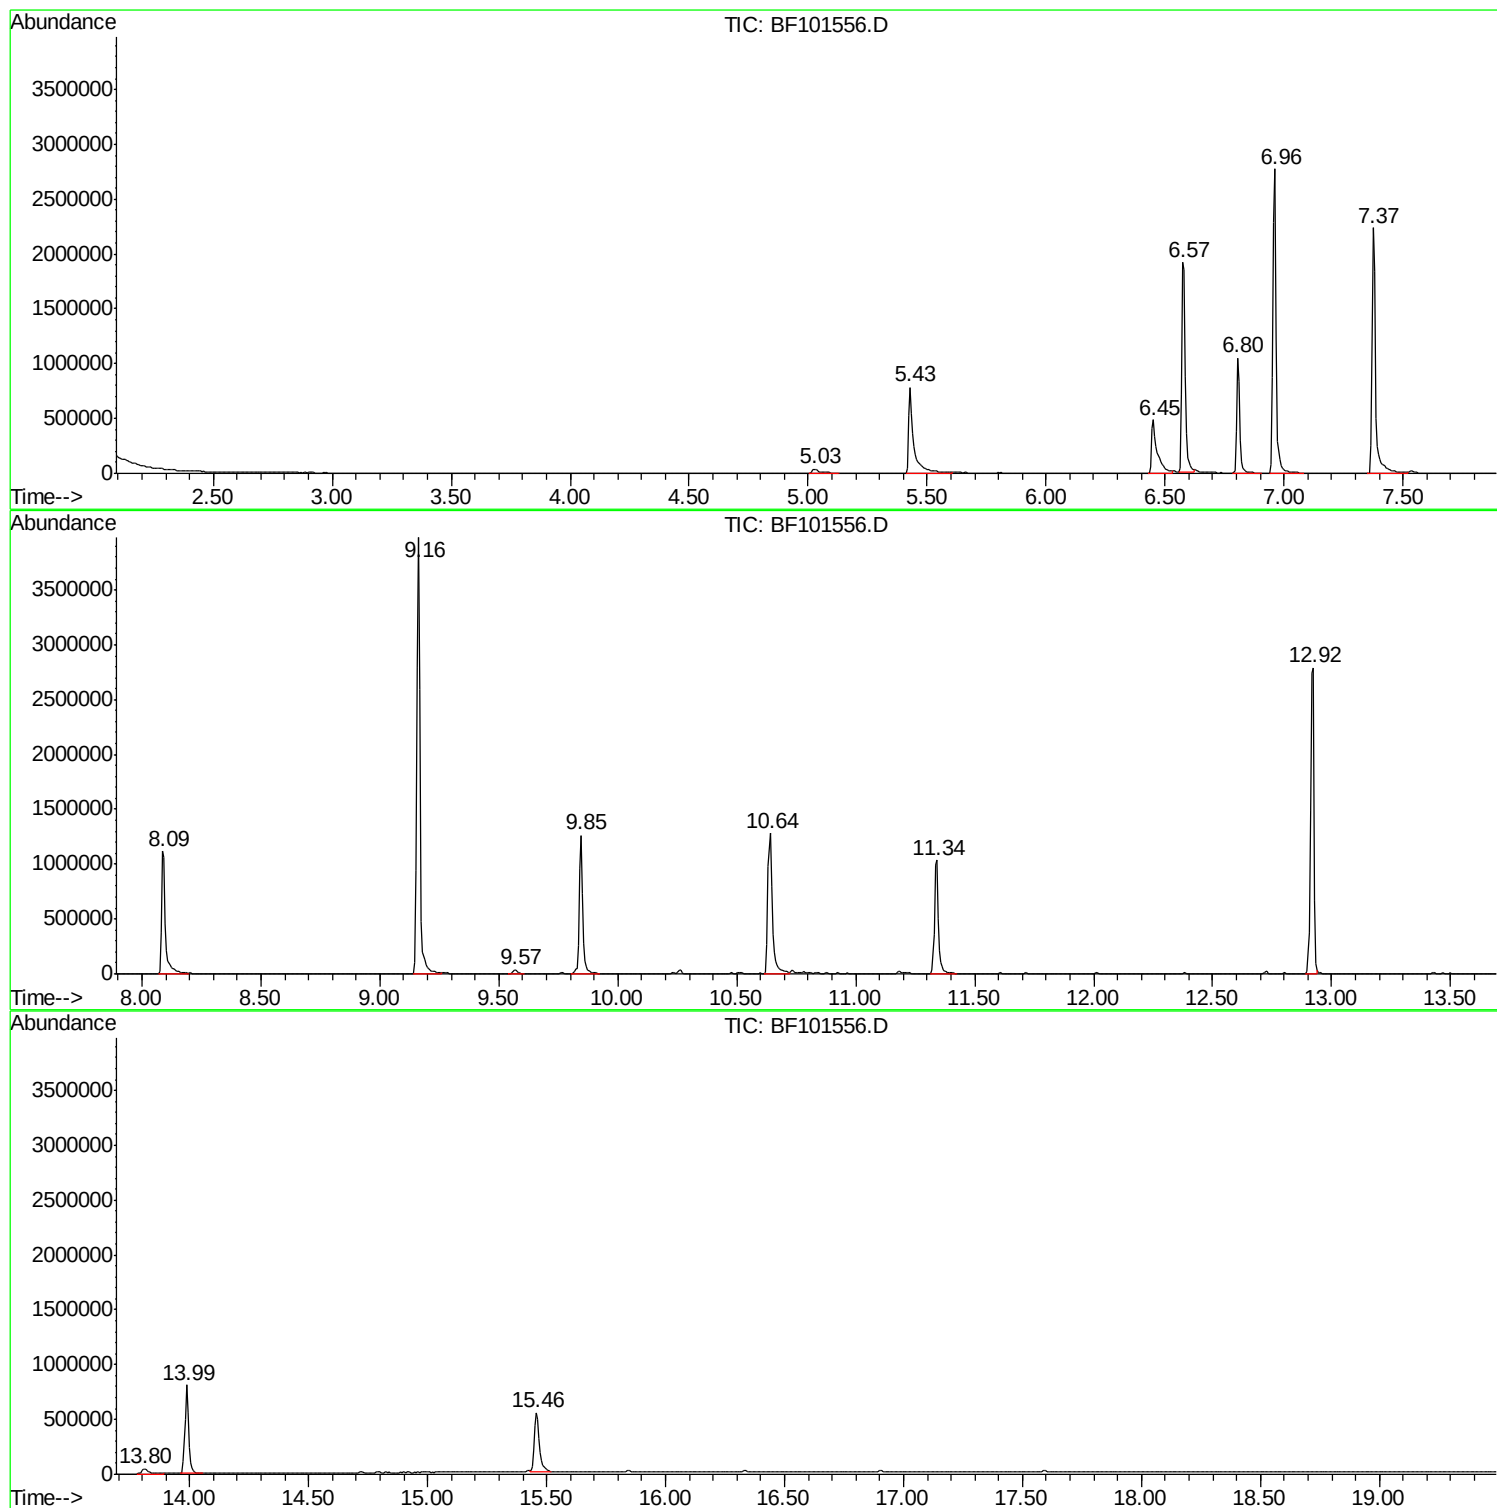

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101556.D
Acq On : 20 Dec 2017 7:38
Operator : SJ/JU
Sample : I6956-08
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121417-JETT-E-D-S










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.57 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.57	42.25 ng	2103680	1,4-Dichlorobenzene-d4	6.80

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

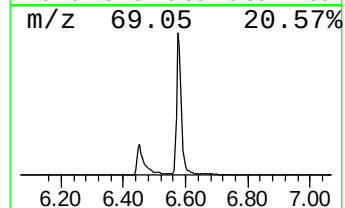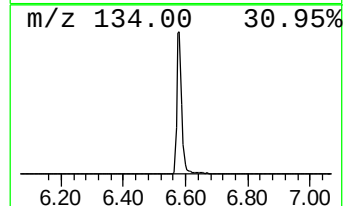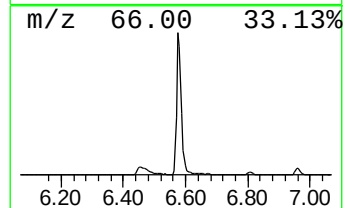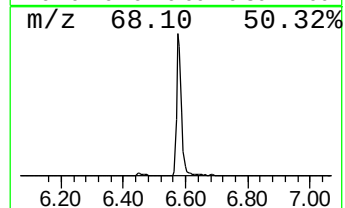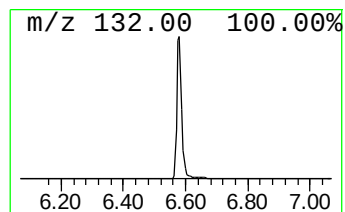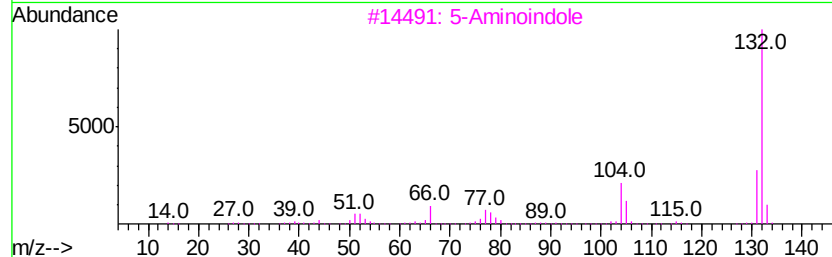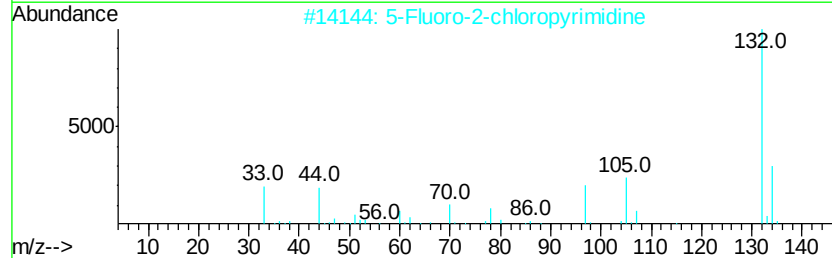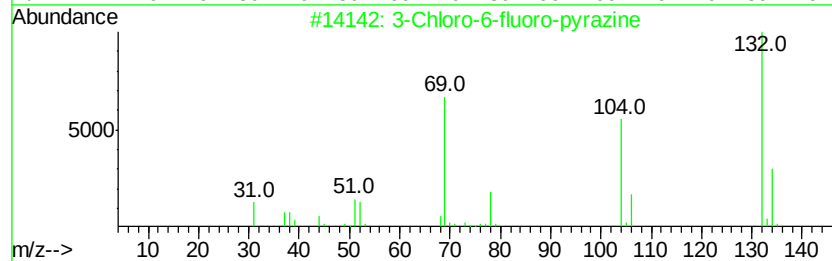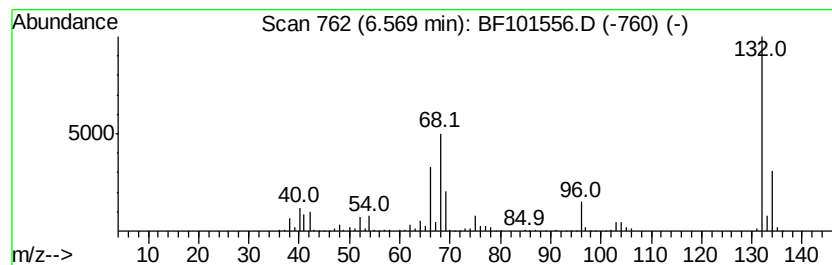

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121917\
Data File : BF101556.D
Acq On : 20 Dec 2017 7:38
Operator : SJ/JU
Sample : I6956-08
Misc :
ALS Vial : 39 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
121417-JETT-E-D-S

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Heptafluorobutyric acid, pe... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.		
13.80	2.48 ng	106392	Chrysene-d12	13.99		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94
2		Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	94
3		Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	94
4		Bromoacetic acid, hexadecyl ester	362	C18H35BrO2	005454-48-8	94
5		Acetic acid, chloro-, hexadecyl ...	318	C18H35ClO2	052132-58-8	93

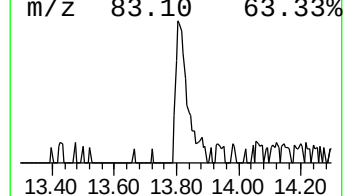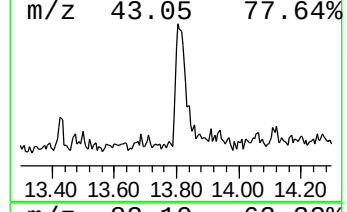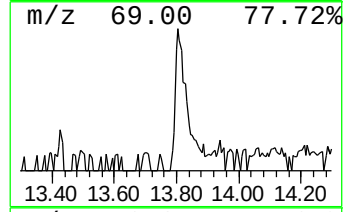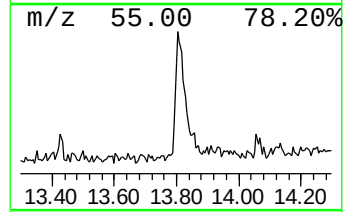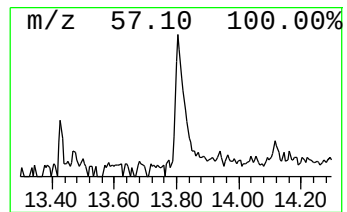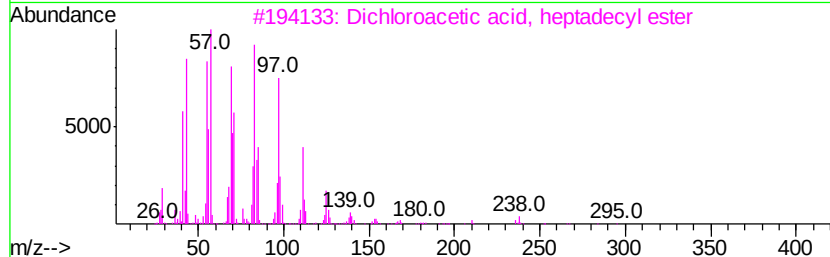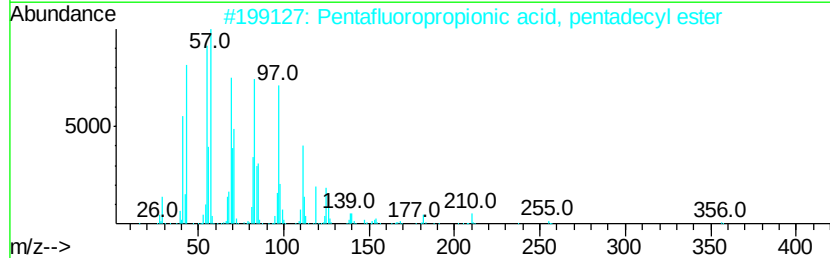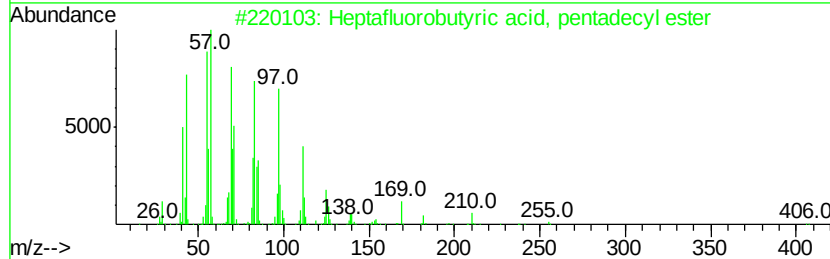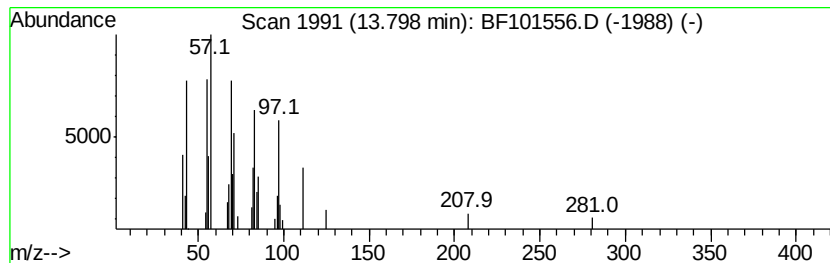

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF121917\
Data File : BF101556.D
Acq On : 20 Dec 2017 7:38
Operator : SJ/JU
Sample : I6956-08
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121417-JETT-E-D-S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.57	6.57	42.3	ng	2103680	1	6.80	995850	20.0
Heptafluorobutyri...	13.80	2.5	ng	106392	5	13.99	857227	20.0