


Data Path : Z:\HPCHEM1\BNA_F\Data\BF121917\
 Data File : BF101516.D
 Acq On : 19 Dec 2017 11:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 18 15:38:59 2017

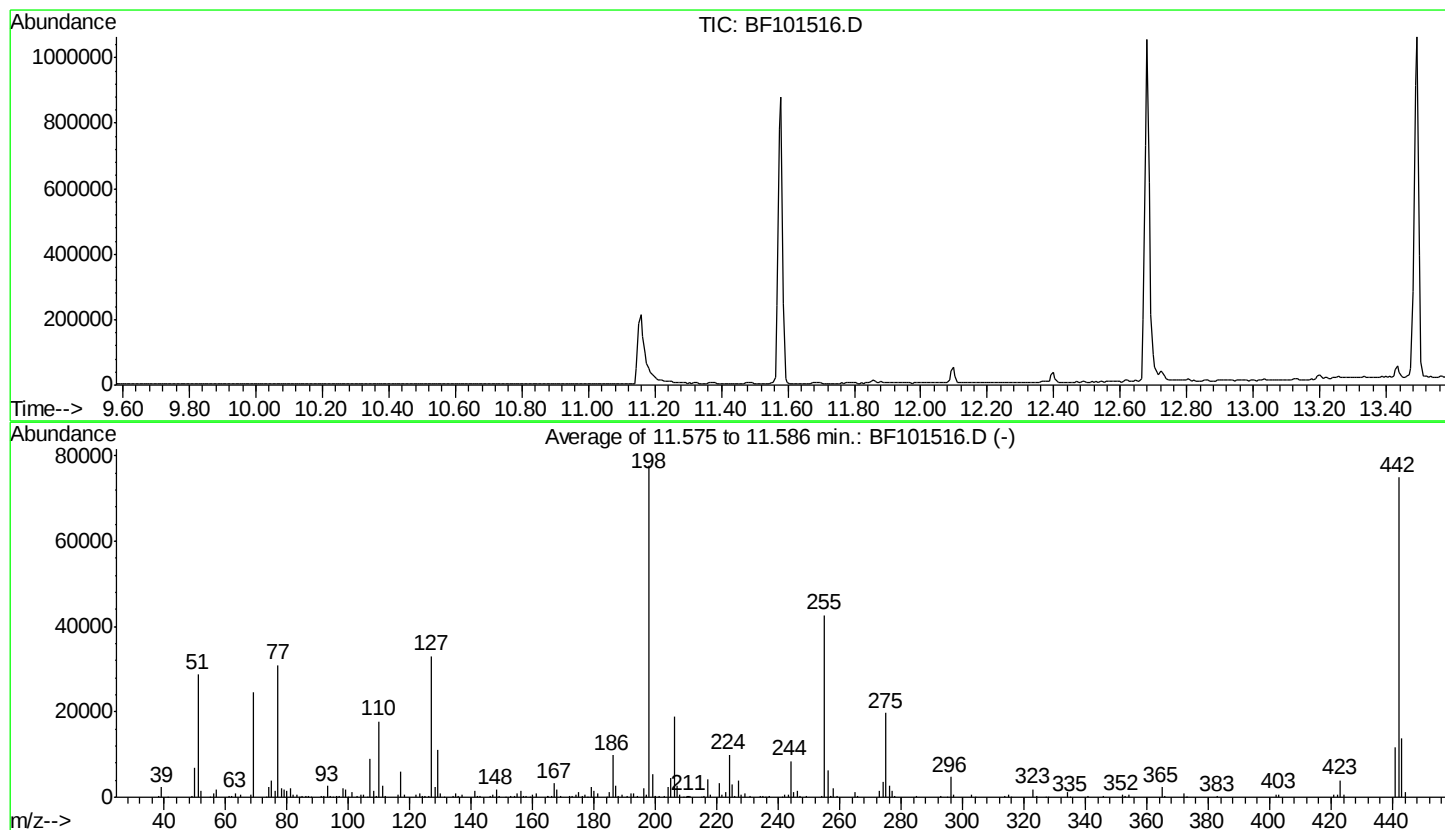

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	28701	PASS
68	69	0.00	2	1.9	467	PASS
69	198	0.00	100	31.7	24637	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.6	33098	PASS
197	198	0.00	2	0.7	572	PASS
198	198	100	100	100.0	77698	PASS
199	198	5	9	6.9	5378	PASS
275	198	10	60	25.3	19694	PASS
365	198	1	100	3.0	2357	PASS
441	443	0.01	100	84.1	11731	PASS
442	198	50	100	96.4	74914	PASS
443	442	15	24	18.6	13953	PASS