


Data Path : Z:\HPCHEM1\BNA_F\Data\BF121917\
Data File : BF101541.D
Acq On : 20 Dec 2017 00:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 18 15:38:59 2017

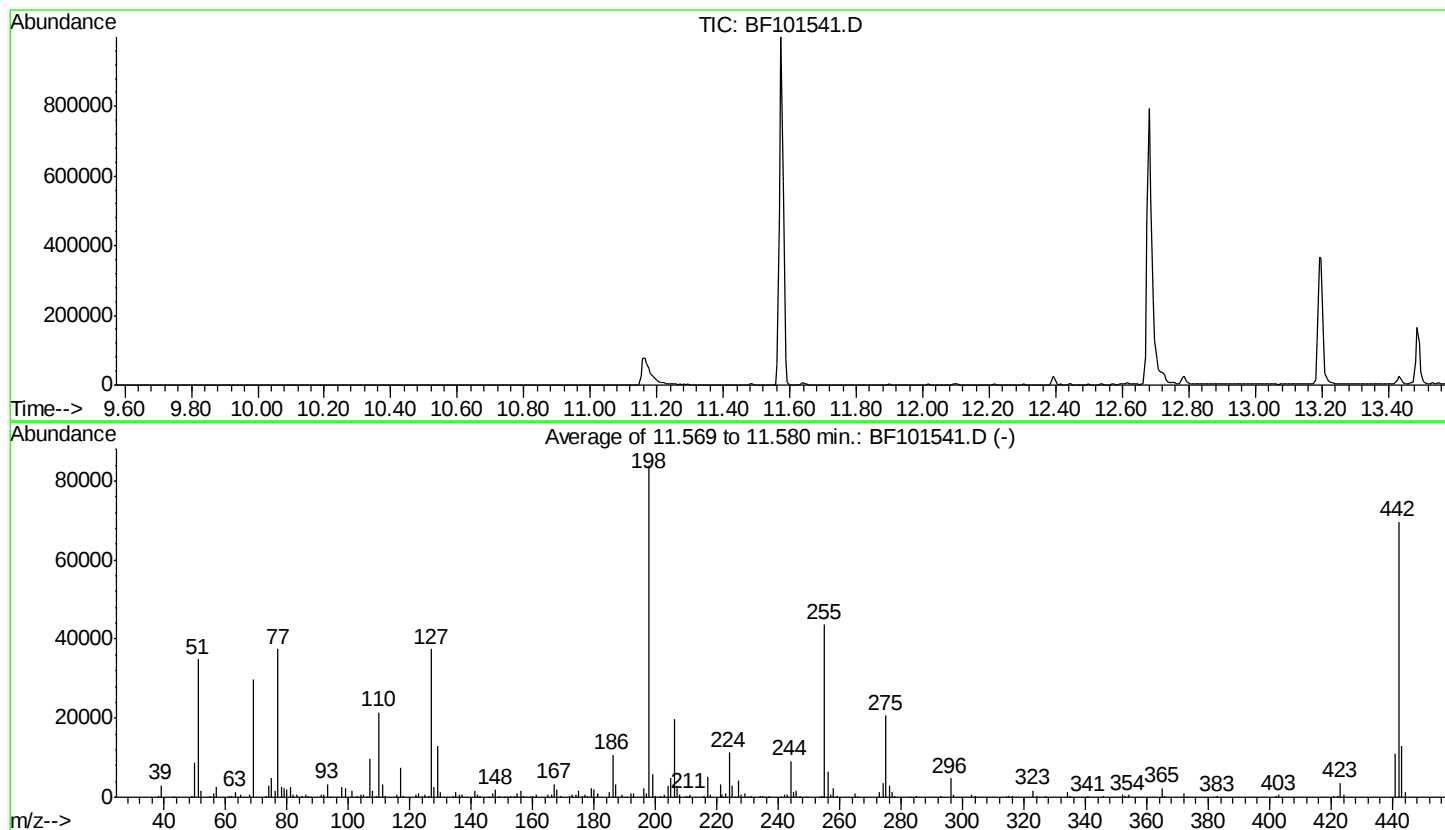

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	34808	PASS
68	69	0.00	2	1.9	566	PASS
69	198	0.00	100	35.6	29848	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.8	37538	PASS
197	198	0.00	2	1.0	840	PASS
198	198	100	100	100.0	83848	PASS
199	198	5	9	7.0	5890	PASS
275	198	10	60	24.5	20579	PASS
365	198	1	100	2.8	2377	PASS
441	443	0.01	100	84.8	11053	PASS
442	198	50	100	83.2	69757	PASS
443	442	15	24	18.7	13031	PASS