
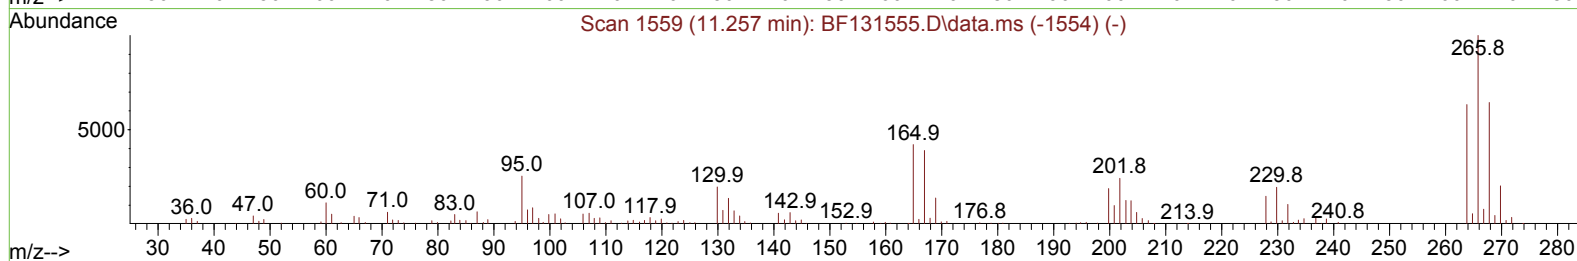
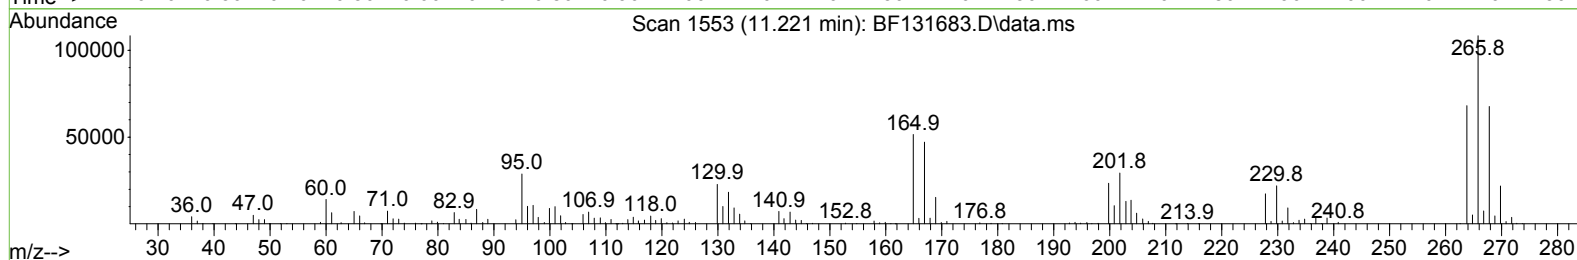


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121922\
Data File : BF131683.D
Acq On : 19 Dec 2022 11:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 03:52:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 00:23:43 2022
Response via : Initial Calibration

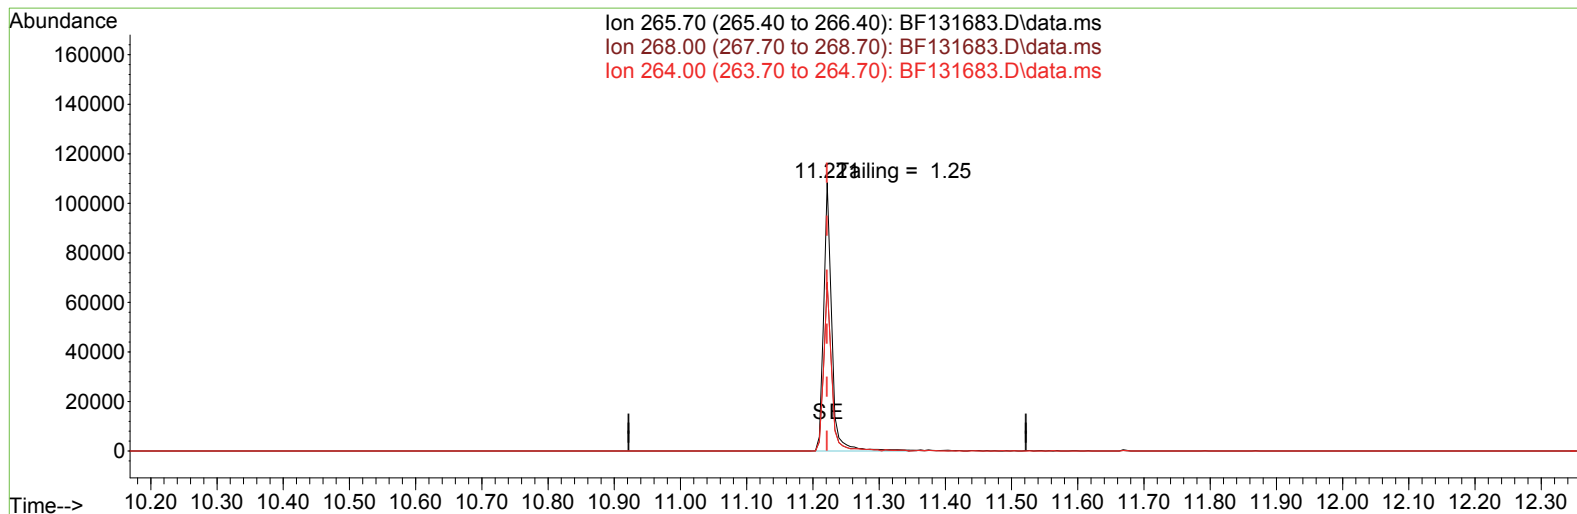

TIC: BF131683.D\data.ms

(70) Pentachlorophenol (C)




11.221min (-0.000) 27120.43 ng

response 92670

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	62.43
264.00	63.40	62.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121922\
Data File : BF131683.D
Acq On : 19 Dec 2022 11:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 03:52:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 00:23:43 2022
Response via : Initial Calibration

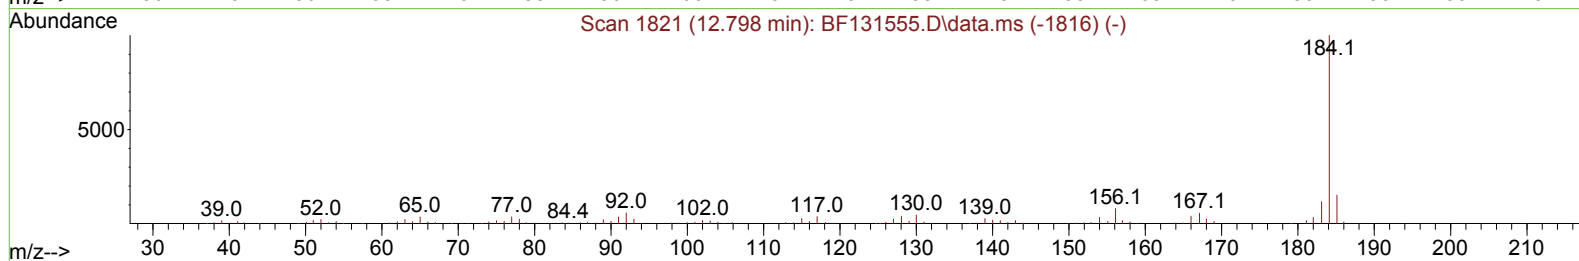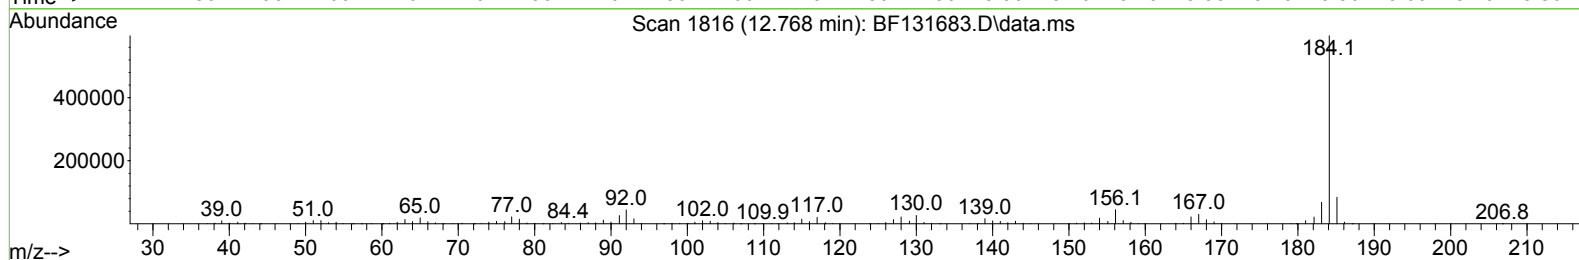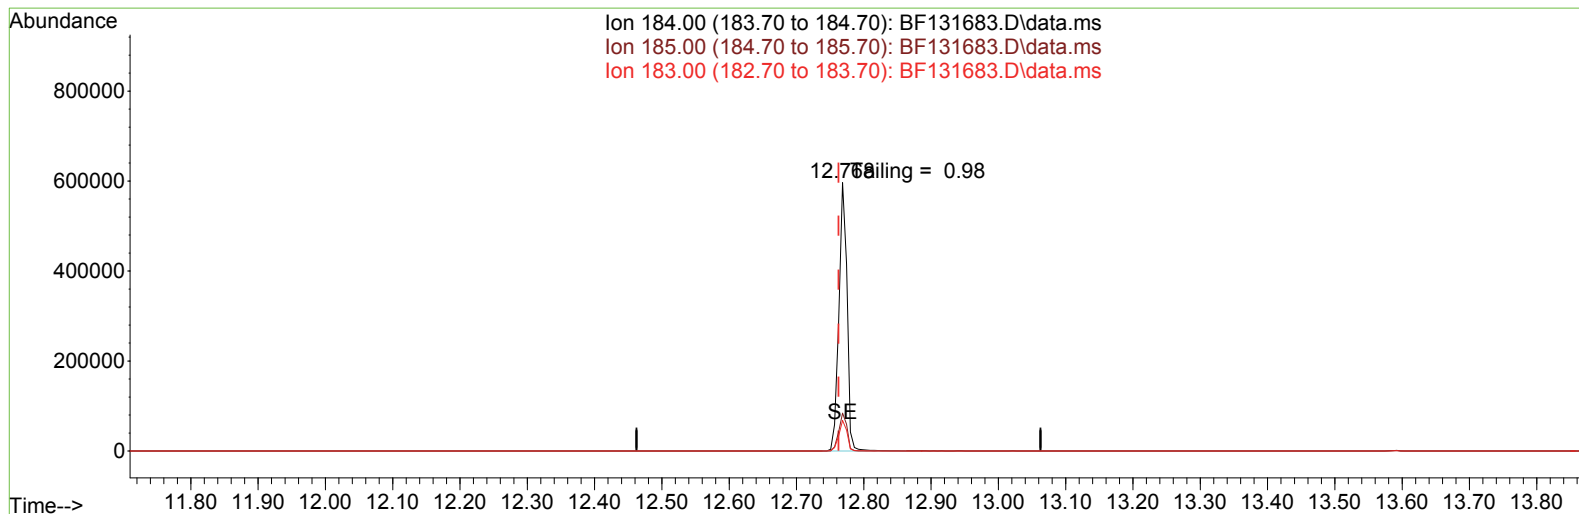

TIC: BF131683.D\data.ms

(77) Benzidine

12.768min (+ 0.006) 0.00 ng m

response 503116

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.14
183.00	11.60	11.41
0.00	0.00	0.00