
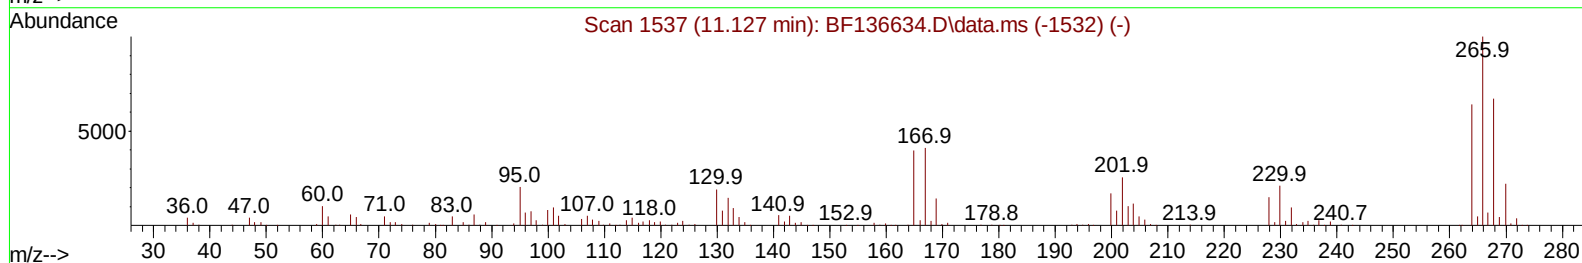
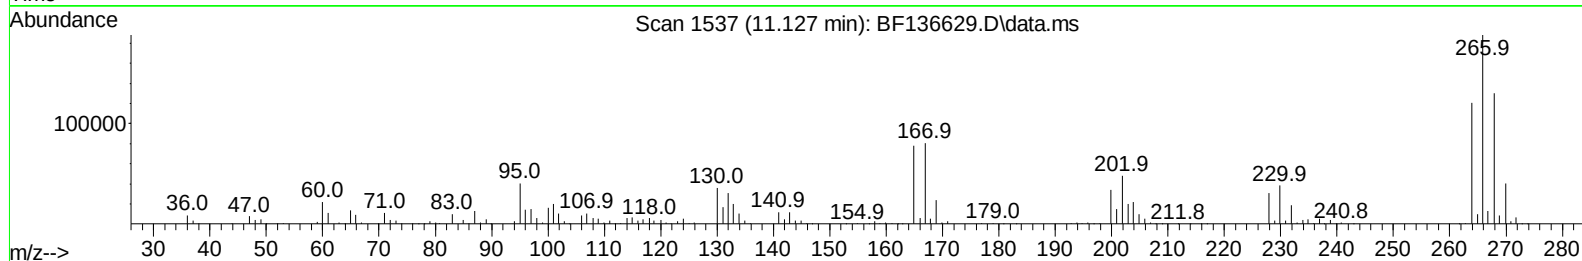


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121923\
Data File : BF136629.D
Acq On : 19 Dec 2023 14:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 16:33:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 00:56:37 2023
Response via : Initial Calibration

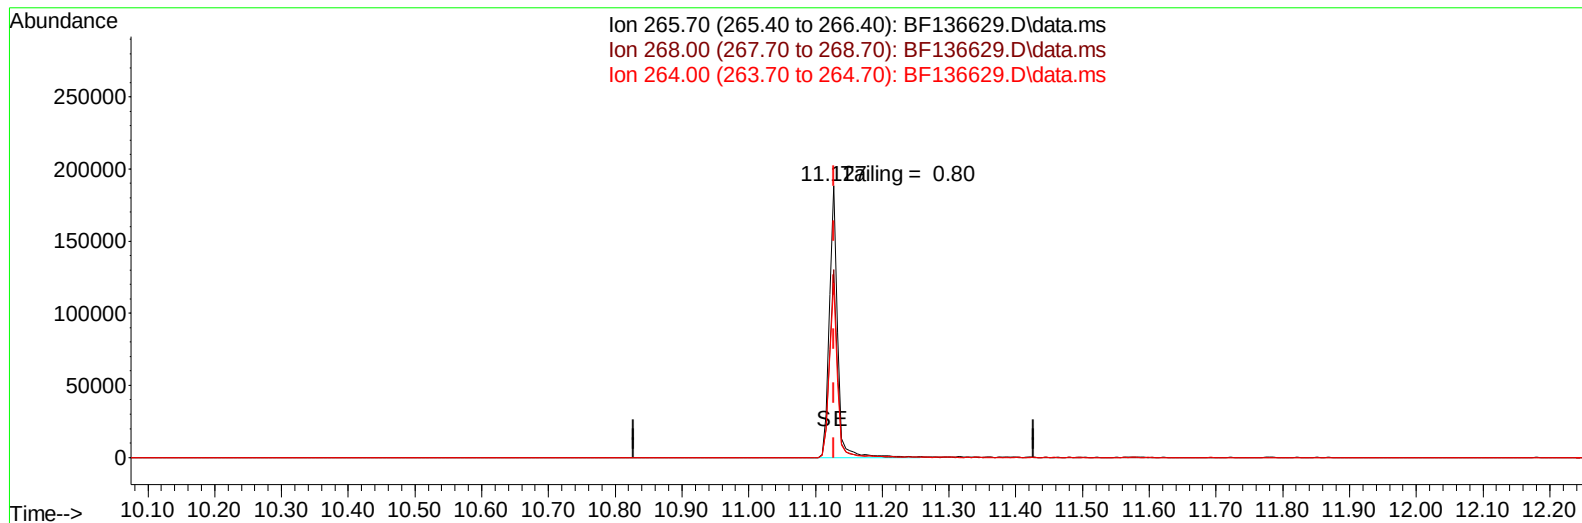

TIC: BF136629.D\data.ms

(70) Pentachlorophenol (C)




11.127min (+ 0.000) 34109.07 ng

response 163488

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	69.09
264.00	65.30	64.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121923\
Data File : BF136629.D
Acq On : 19 Dec 2023 14:30
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 16:33:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 00:56:37 2023
Response via : Initial Calibration

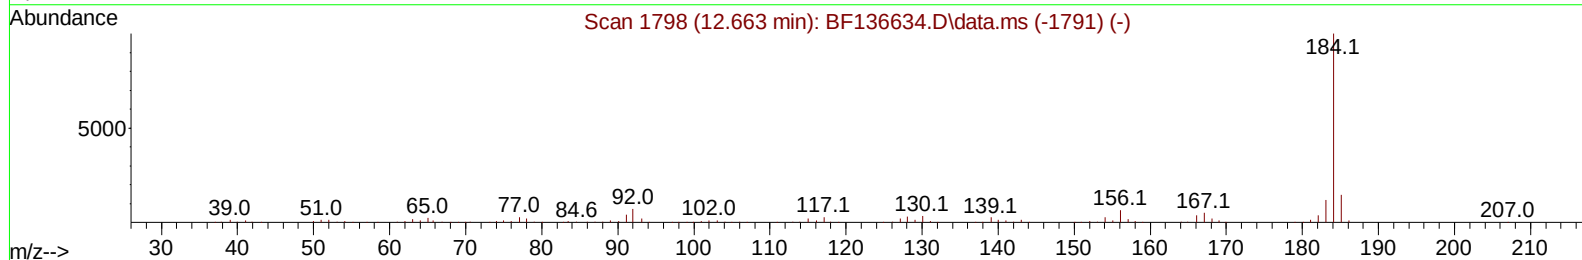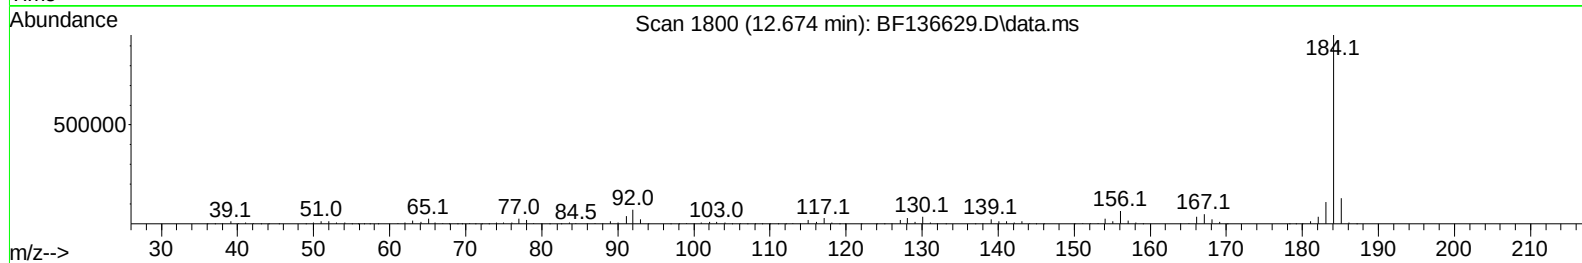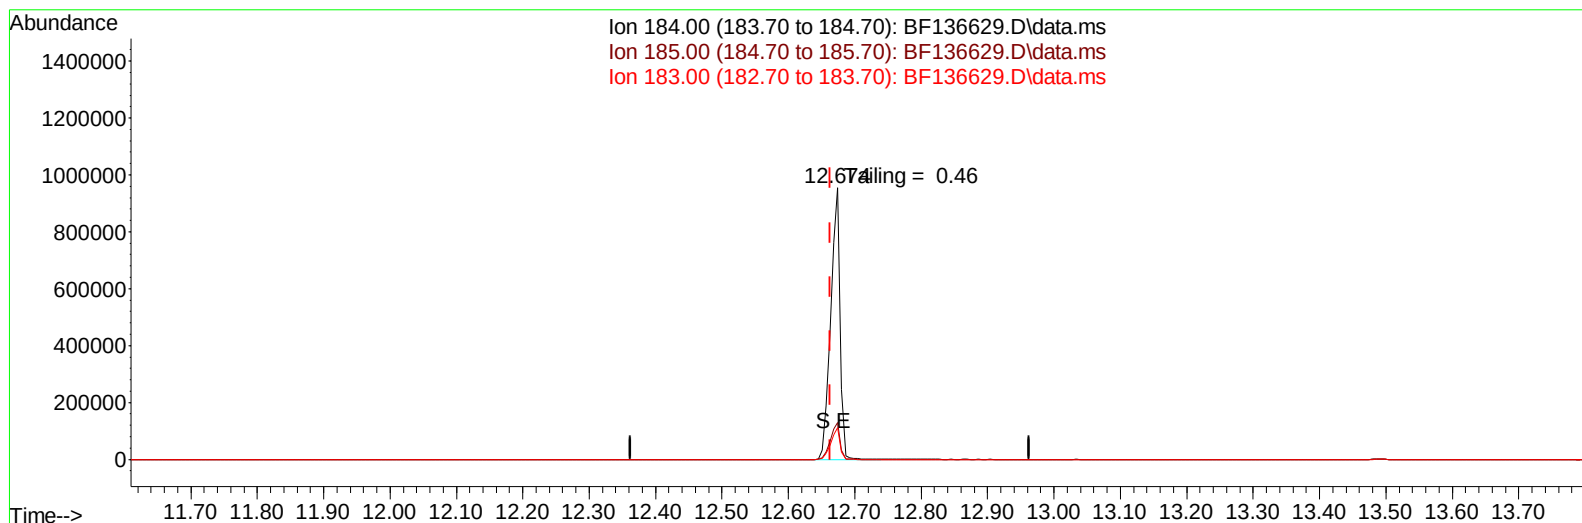

TIC: BF136629.D\data.ms

(77) Benzidine

12.674min (+ 0.012) 0.00 ng

response 939740

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.59
183.00	11.70	11.65
0.00	0.00	0.00