
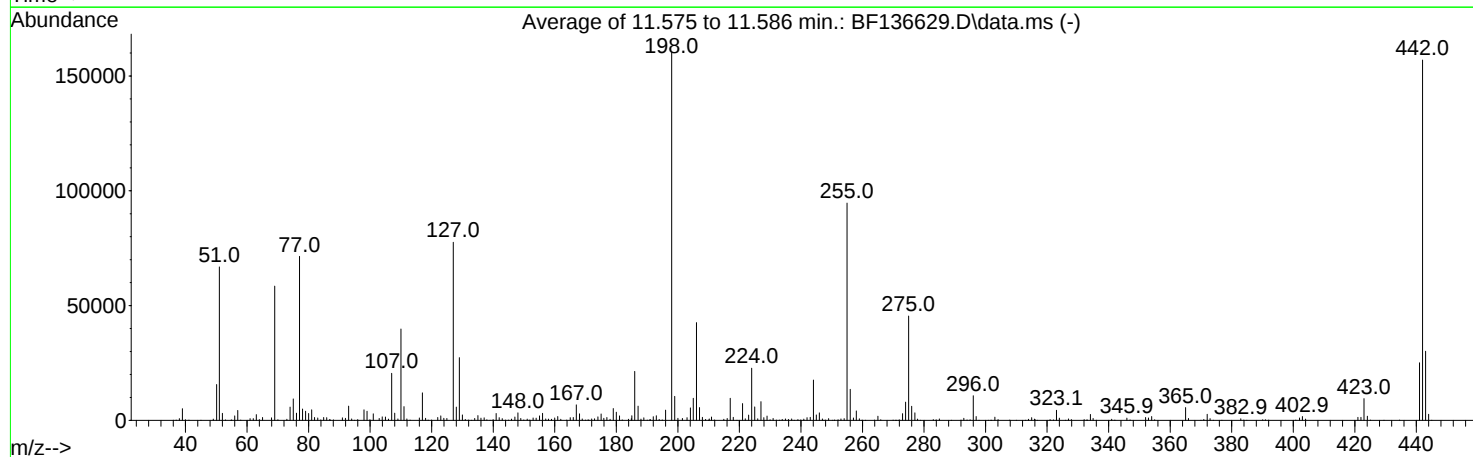


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121923\
 Data File : BF136629.D
 Acq On : 19 Dec 2023 14:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 20 04:16:58 2023

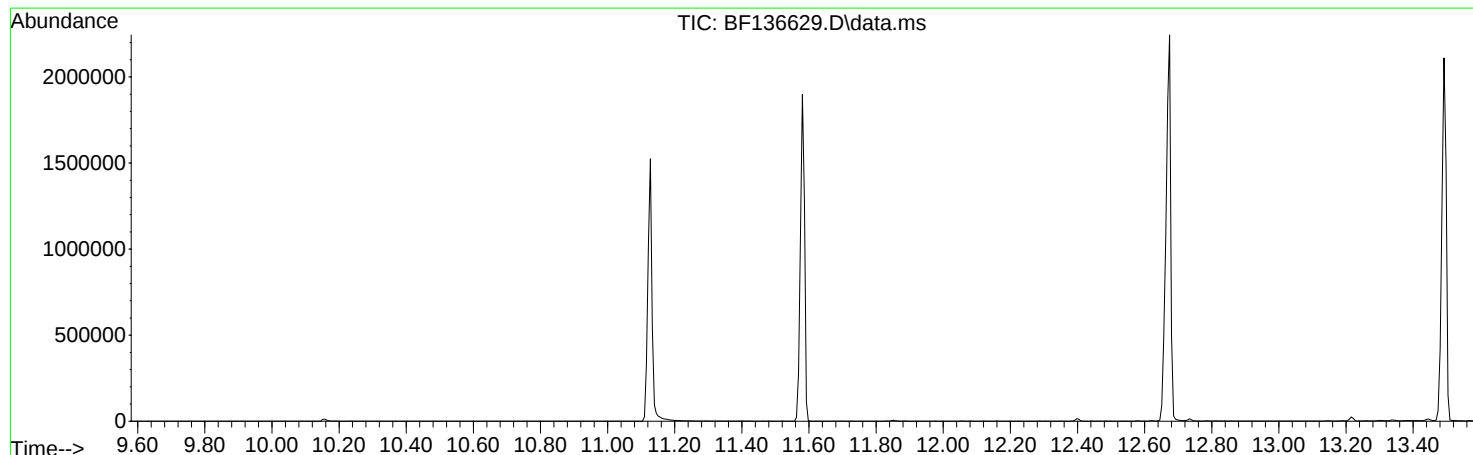




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	66829	PASS
68	69	0.00	2	1.9	1095	PASS
69	198	0.00	100	36.5	58443	PASS
70	69	0.00	2	0.5	277	PASS
127	198	10	80	48.4	77552	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	160224	PASS
199	198	5	9	6.5	10429	PASS
275	198	10	60	28.3	45421	PASS
365	198	1	100	3.5	5550	PASS
441	198	0.01	100	15.6	25066	PASS
442	442	50	100	100.0	156949	PASS
443	442	15	24	19.2	30101	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121923\
Data File : BF136629.D
Acq On : 19 Dec 2023 14:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 19 16:33:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 00:56:37 2023
Response via : Initial Calibration

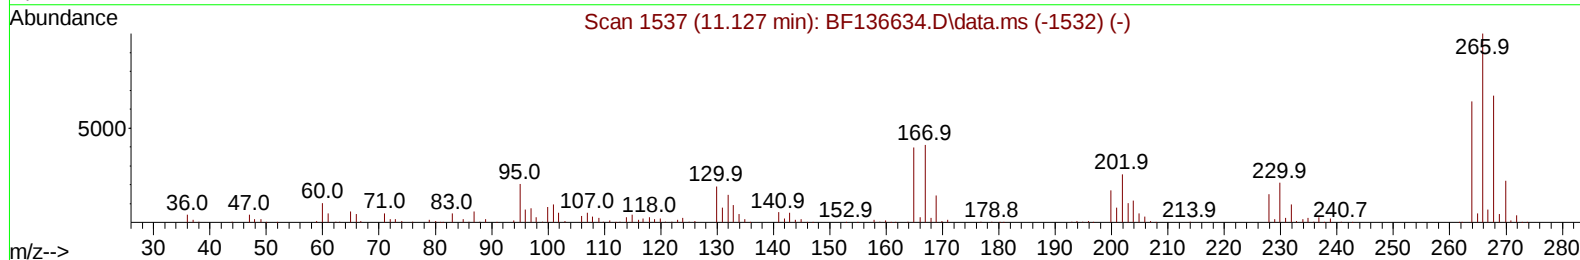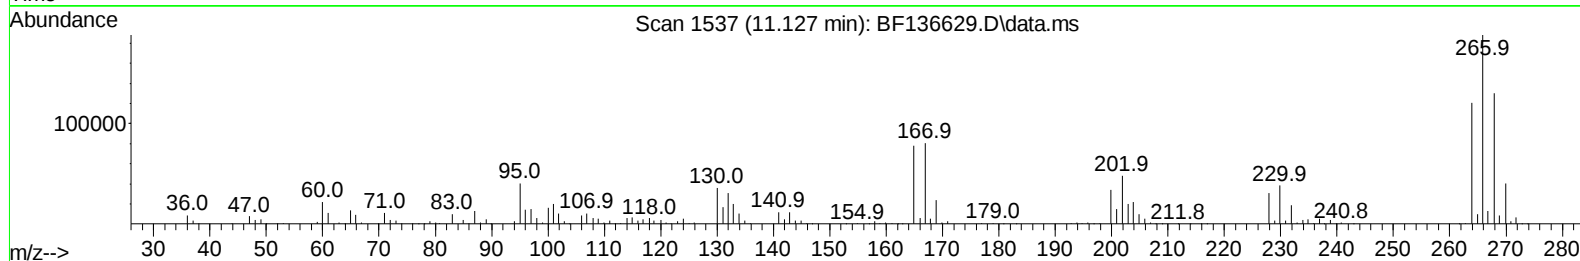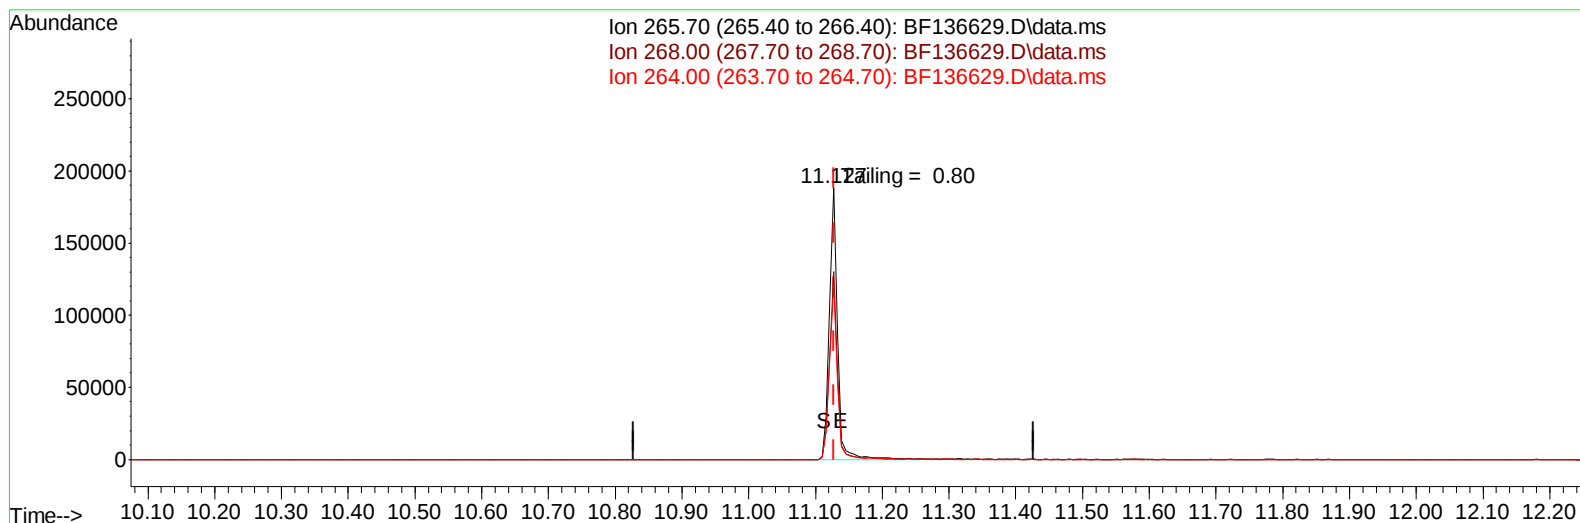

TIC: BF136629.D\data.ms

(70) Pentachlorophenol (C)

11.127min (+ 0.000) 34109.07 ng




response 163488

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	69.09
264.00	65.30	64.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121923\
Data File : BF136629.D
Acq On : 19 Dec 2023 14:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 19 16:33:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 00:56:37 2023
Response via : Initial Calibration

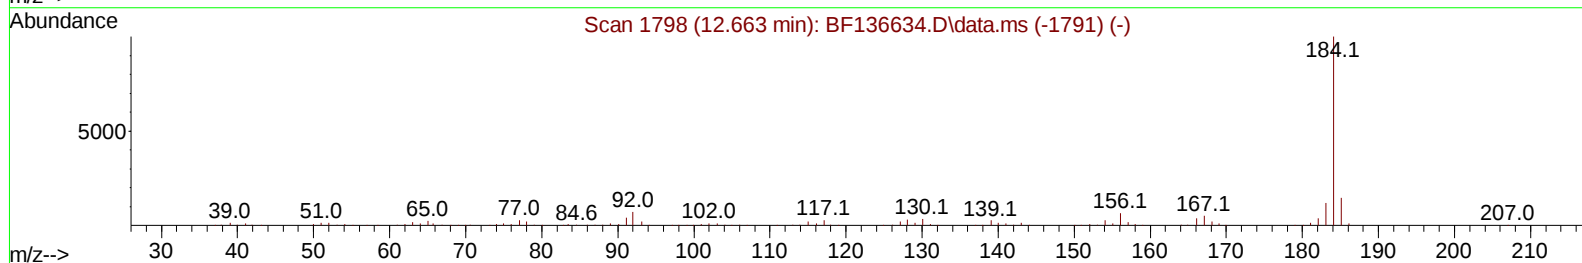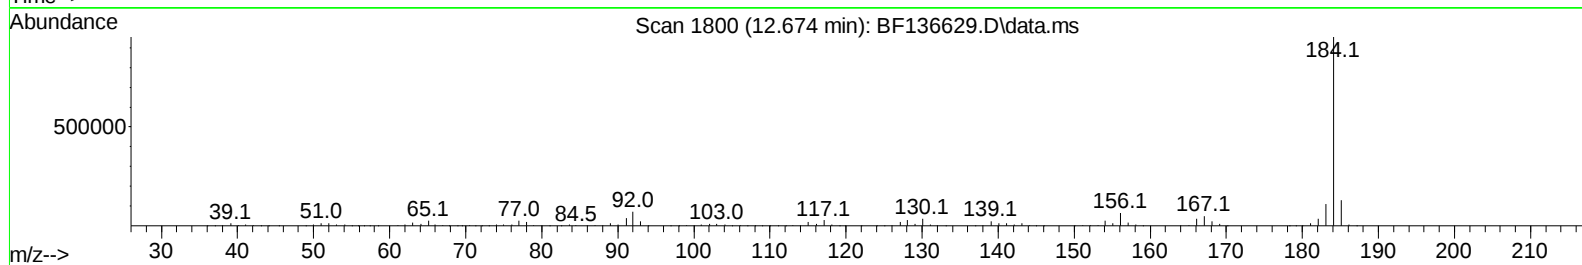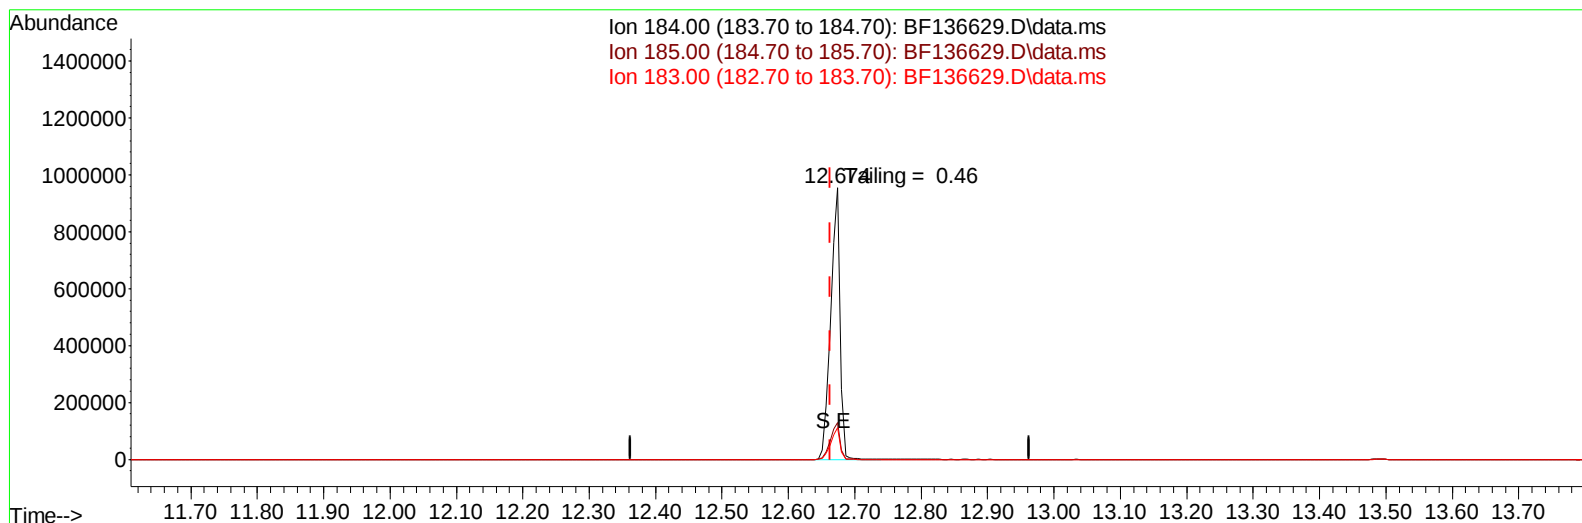

TIC: BF136629.D\data.ms

(77) Benzidine

12.674min (+ 0.012) 0.00 ng

response 939740

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.59
183.00	11.70	11.65
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/19/2023	BNA_F	<u>BF136629.D</u>
Compound Name	Response	Retention Time
DDT	405758	13.492
DDD	5277	13.216
DDE	179	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5456	411214	1.33

Instrument :
BNA_F
ClientSampleId :
DFTPP