
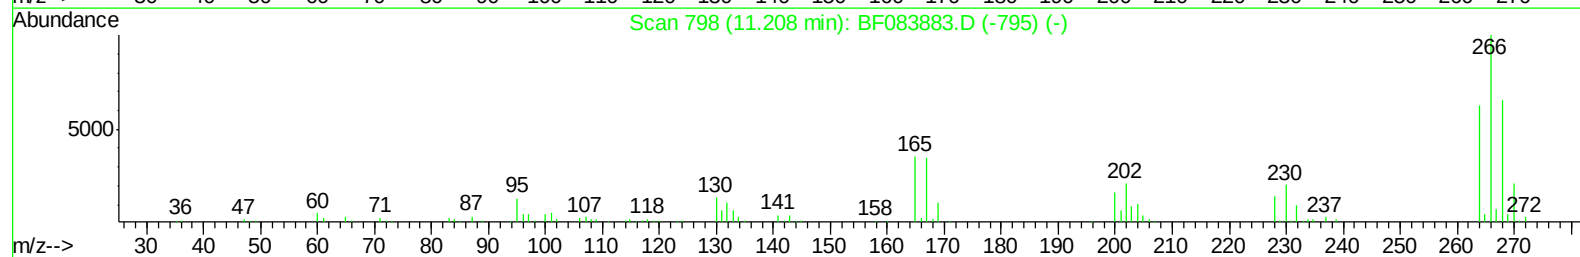
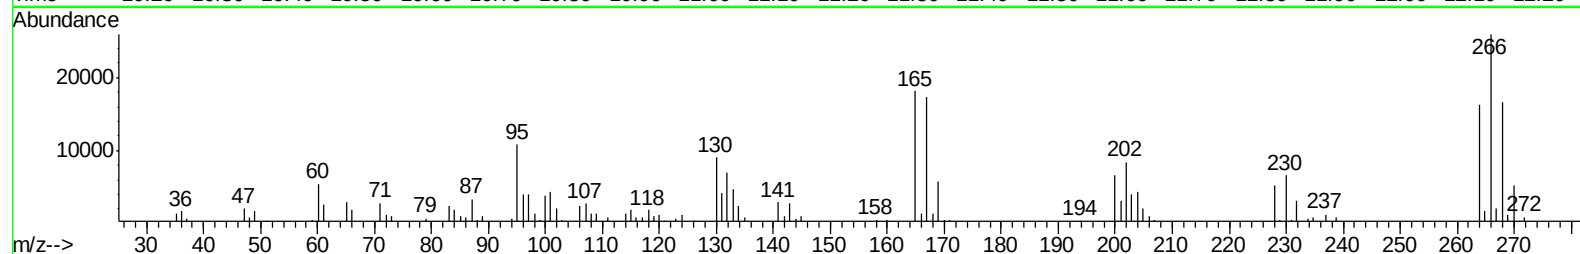


Data Path : Z:\HPCHEM1\BNA_F\Data\BF122015\
Data File : BF083948.D
Acq On : 19 Dec 2015 12:14
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 07:42:42 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 18 14:23:22 2015
Response via : Initial Calibration

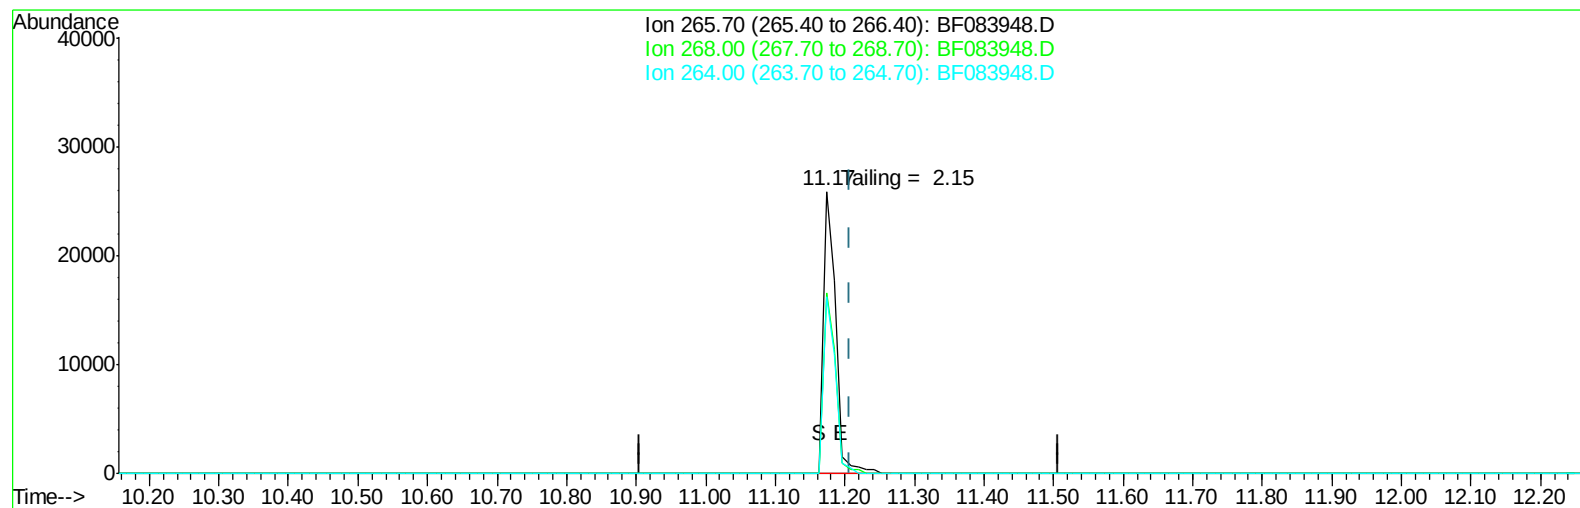

TIC: BF083948.D

(69) Pentachlorophenol (C)

11.174min (-0.033) 20823.65ng

response 32389

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	64.33
264.00	62.70	62.65
0.00	0.00	0.00

