
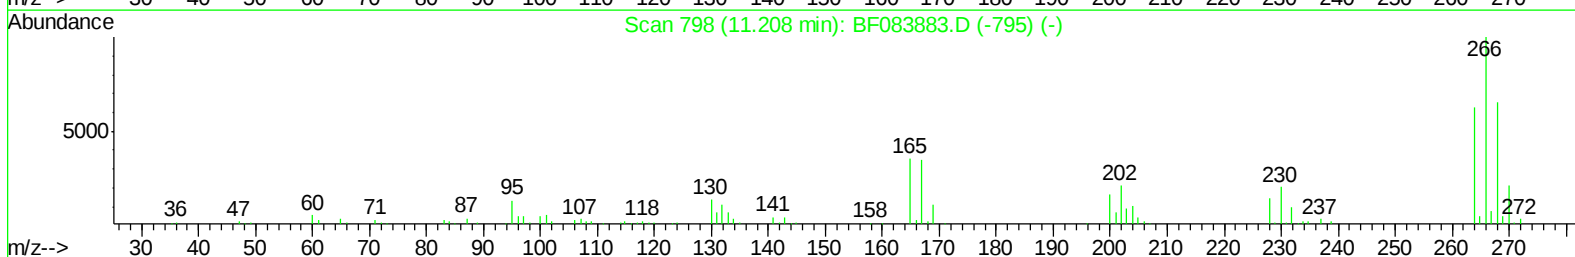
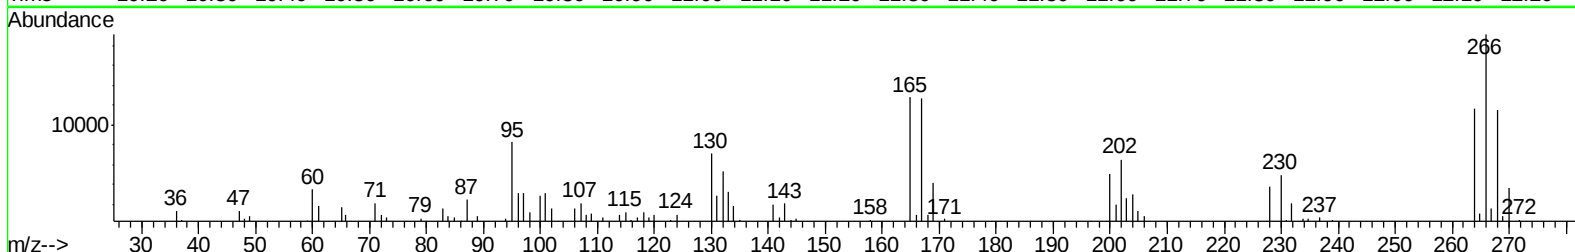


Data Path : Z:\HPCHEM1\BNA_F\Data\BF122015\
Data File : BF083974.D
Acq On : 20 Dec 2015 2:12
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 07:43:50 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 18 14:23:22 2015
Response via : Initial Calibration

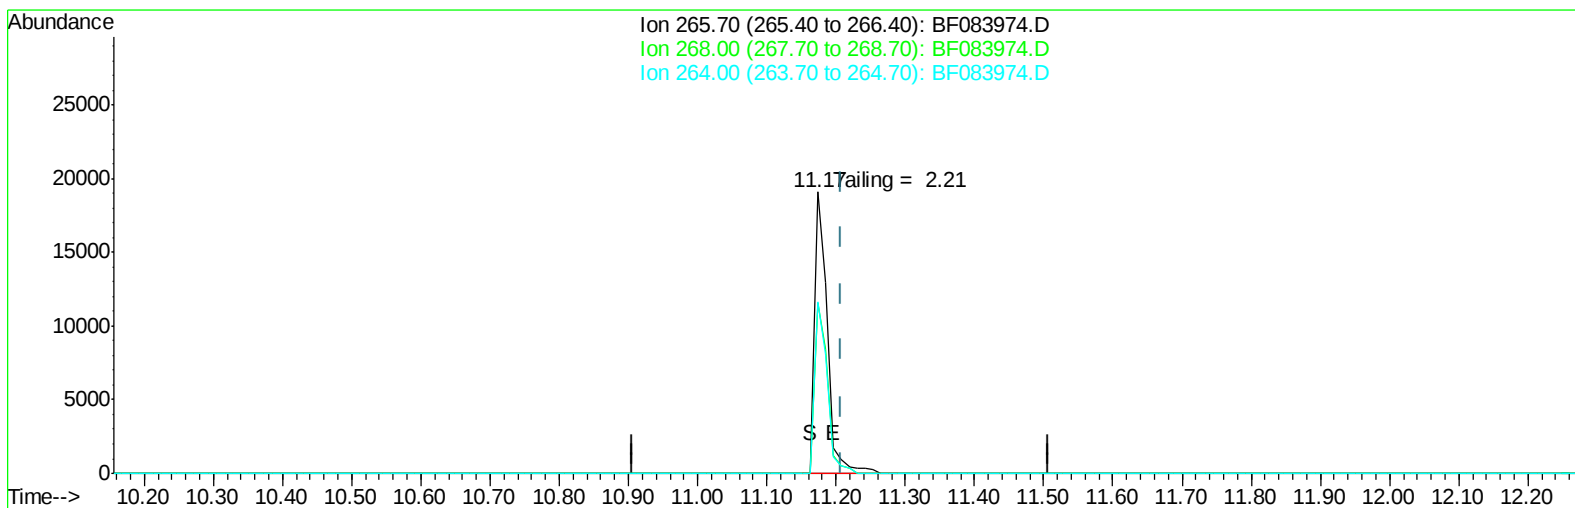

TIC: BF083974.D

(69) Pentachlorophenol (C)




11.173min (-0.034) 0.00ng

response 24816

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	60.52
264.00	62.70	61.05
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF122015\
Data File : BF083974.D
Acq On : 20 Dec 2015 2:12
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 07:43:50 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 18 14:23:22 2015
Response via : Initial Calibration

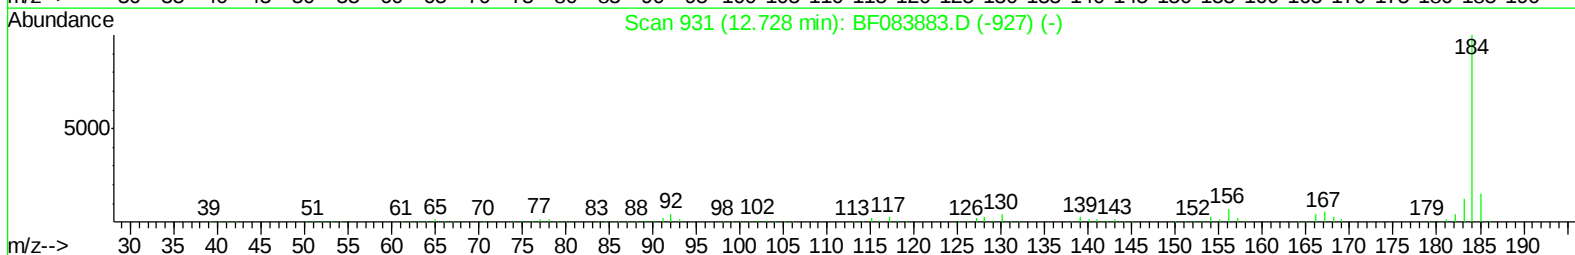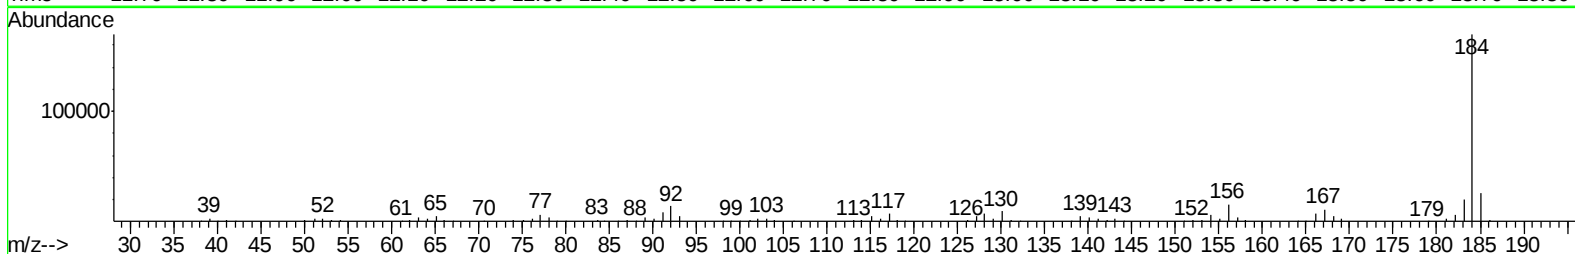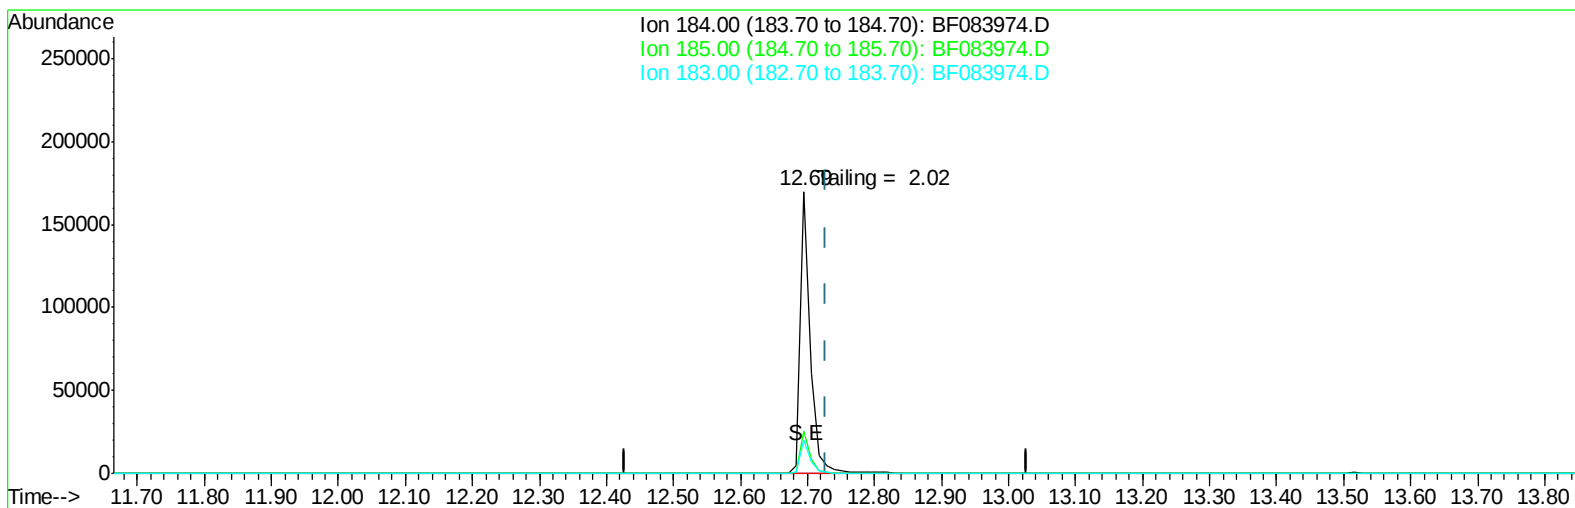

TIC: BF083974.D

(76) Benzidine

12.694min (-0.034) 0.00ng

response 177093

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.04
183.00	12.30	11.91
0.00	0.00	0.00