


Data Path : Z:\HPCHEM1\BNA F\DATA\BF122015\  
 Data File : BF083948.D  
 Acq On : 19 Dec 2015 12:14  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF121815.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Dec 18 14:23:22 2015

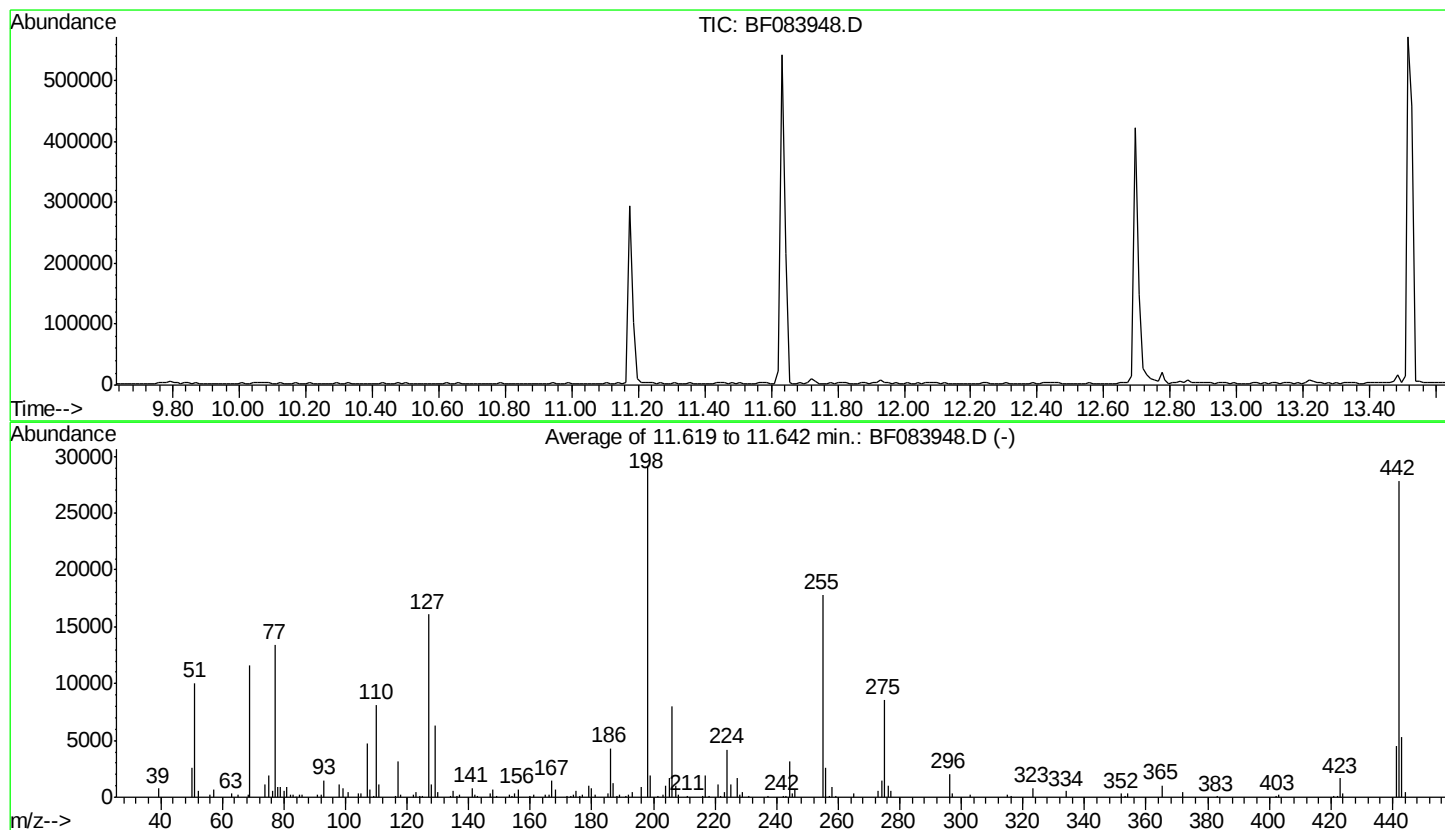

AutoFind: Scans 834, 835, 836; Background Corrected with Scan 831

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 34.5      | 10072   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 198     | PASS             |
| 69          | 198          | 0.00         | 100          | 39.7      | 11576   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 55.1      | 16075   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 29182   | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 1904    | PASS             |
| 275         | 198          | 10           | 60           | 29.4      | 8565    | PASS             |
| 365         | 198          | 1            | 100          | 3.5       | 1018    | PASS             |
| 441         | 442          | 0.01         | 24           | 16.1      | 4487    | PASS             |
| 442         | 198          | 50           | 100          | 95.4      | 27850   | PASS             |
| 443         | 442          | 15           | 24           | 18.9      | 5254    | PASS             |