


Data Path : Z:\HPCHEM1\BNA F\DATA\BF122015\
 Data File : BF083974.D
 Acq On : 20 Dec 2015 2:12
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 18 14:23:22 2015

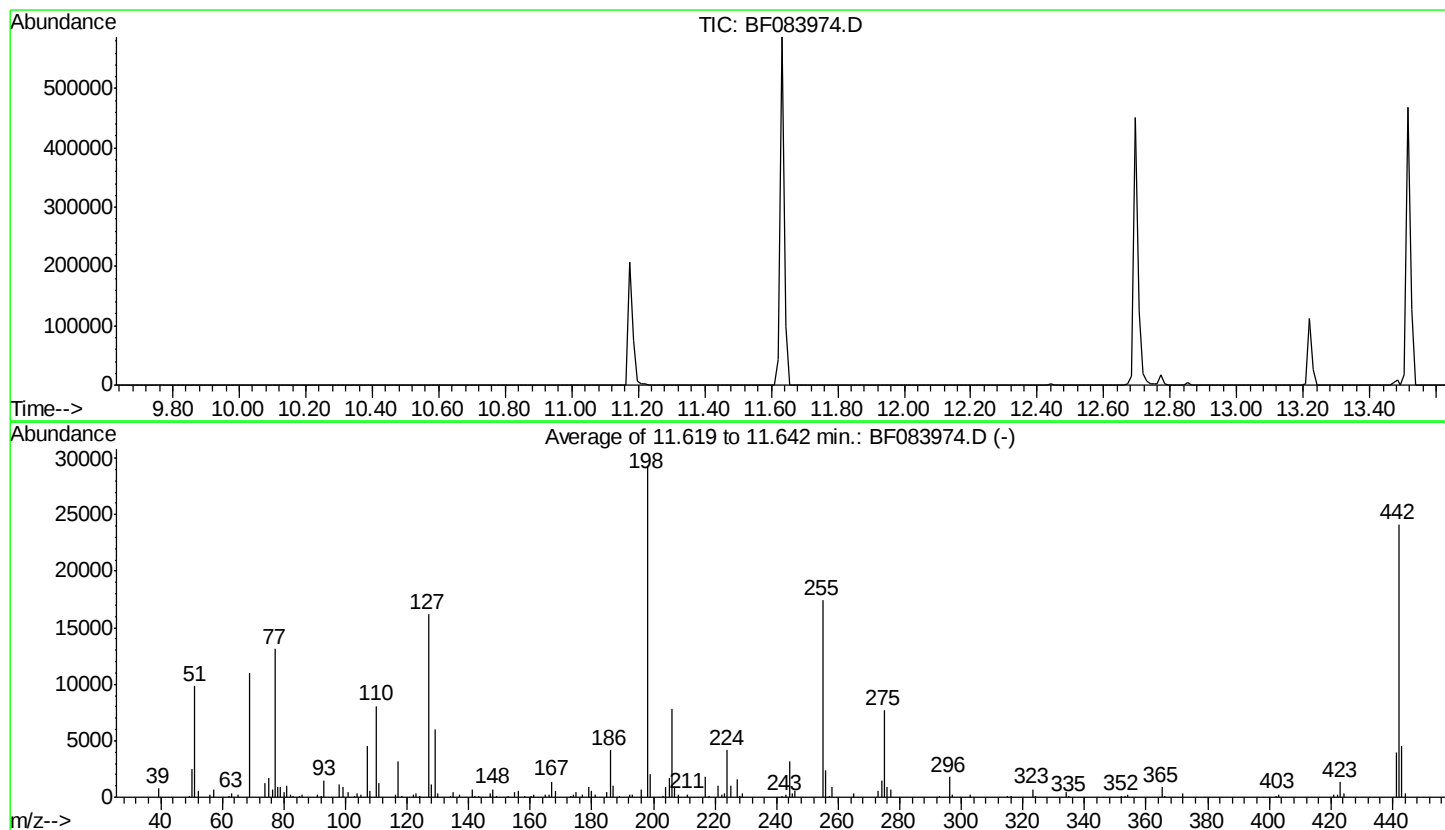

AutoFind: Scans 834, 835, 836; Background Corrected with Scan 831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	9819	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.4	10985	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.1	16154	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	29335	PASS
199	198	5	9	6.8	2000	PASS
275	198	10	60	26.2	7687	PASS
365	198	1	100	3.0	886	PASS
441	442	0.01	24	16.3	3931	PASS
442	198	50	100	82.0	24069	PASS
443	442	15	24	18.8	4529	PASS