
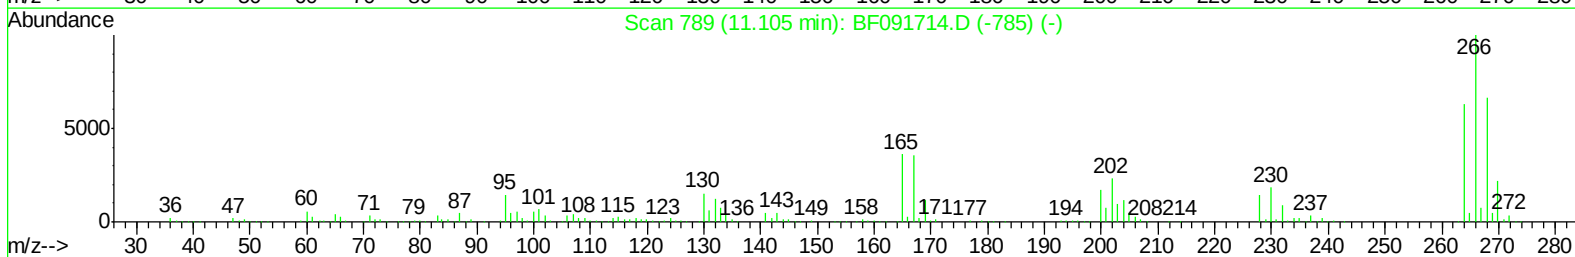
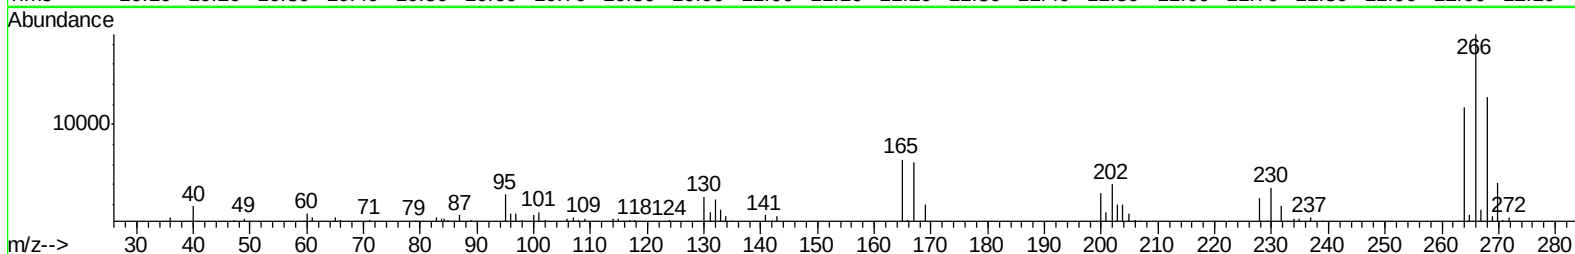


Data Path : Z:\HPCHEM1\BNA_F\Data\BF122016\
Data File : BF091806.D
Acq On : 20 Dec 2016 8:20
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 07:21:57 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 22:53:54 2016
Response via : Initial Calibration

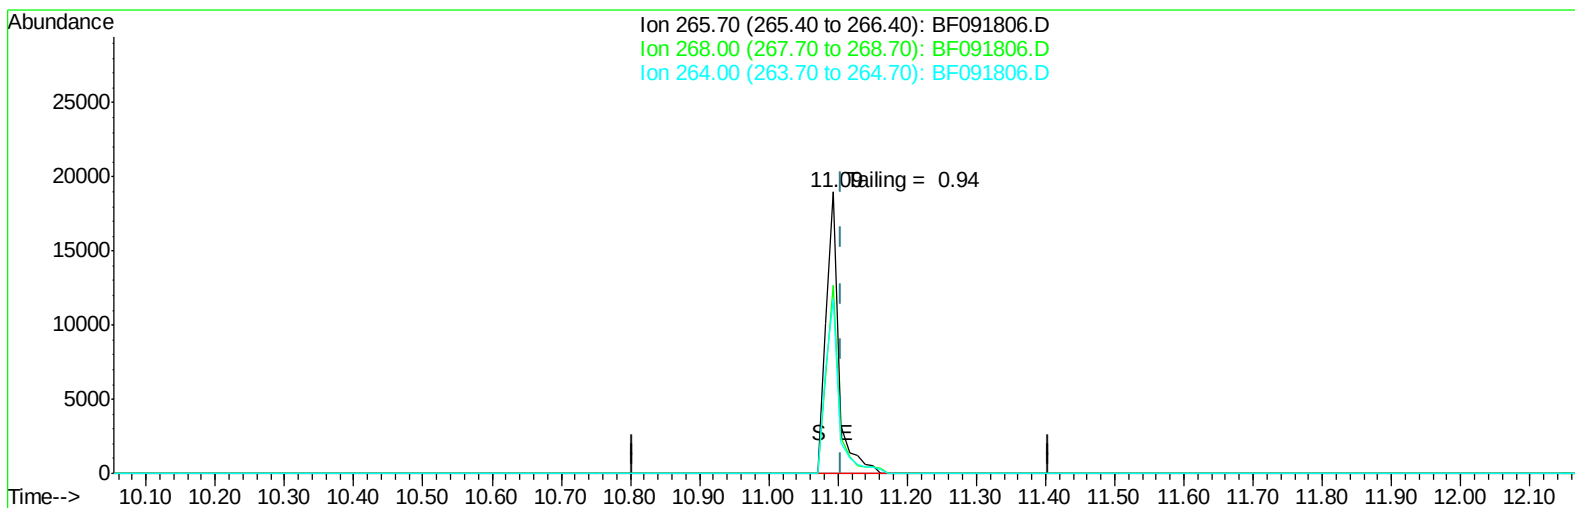

TIC: BF091806.D

(69) Pentachlorophenol (C)




11.094min (-0.011) 0.00ng

response 24671

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	66.78
264.00	62.90	61.67
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF122016\
 Data File : BF091806.D
 Acq On : 20 Dec 2016 8:20
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 07:21:57 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 17 22:53:54 2016
 Response via : Initial Calibration

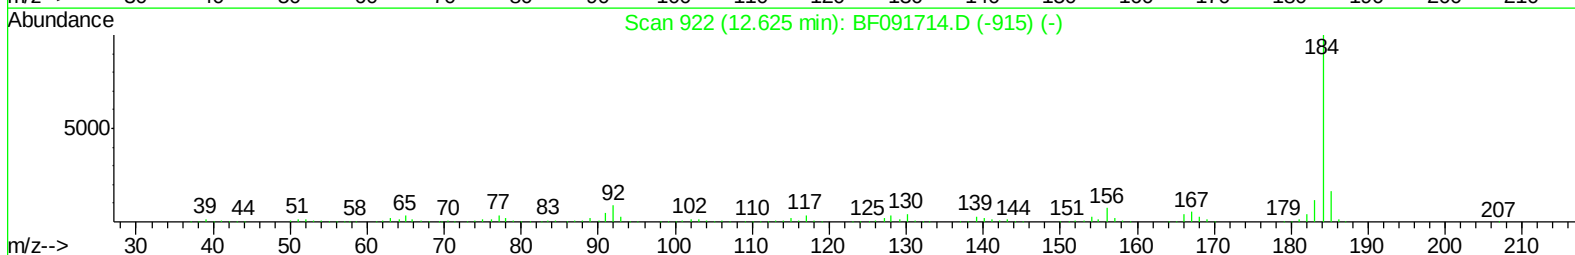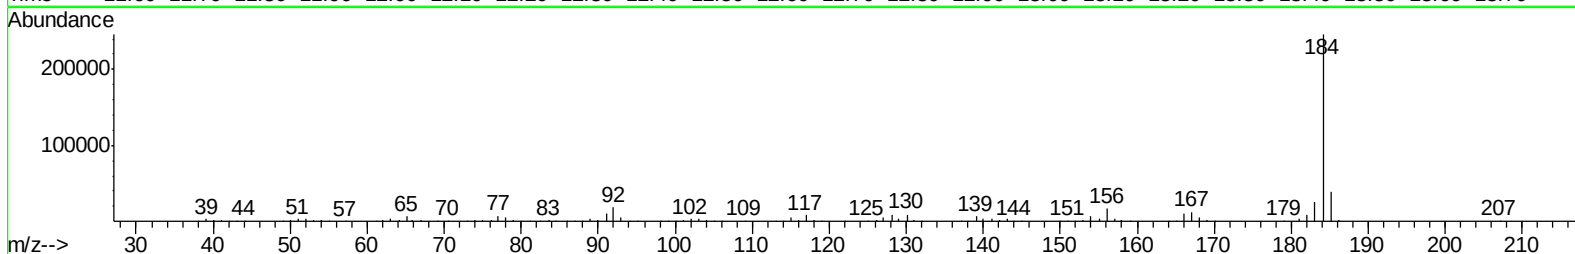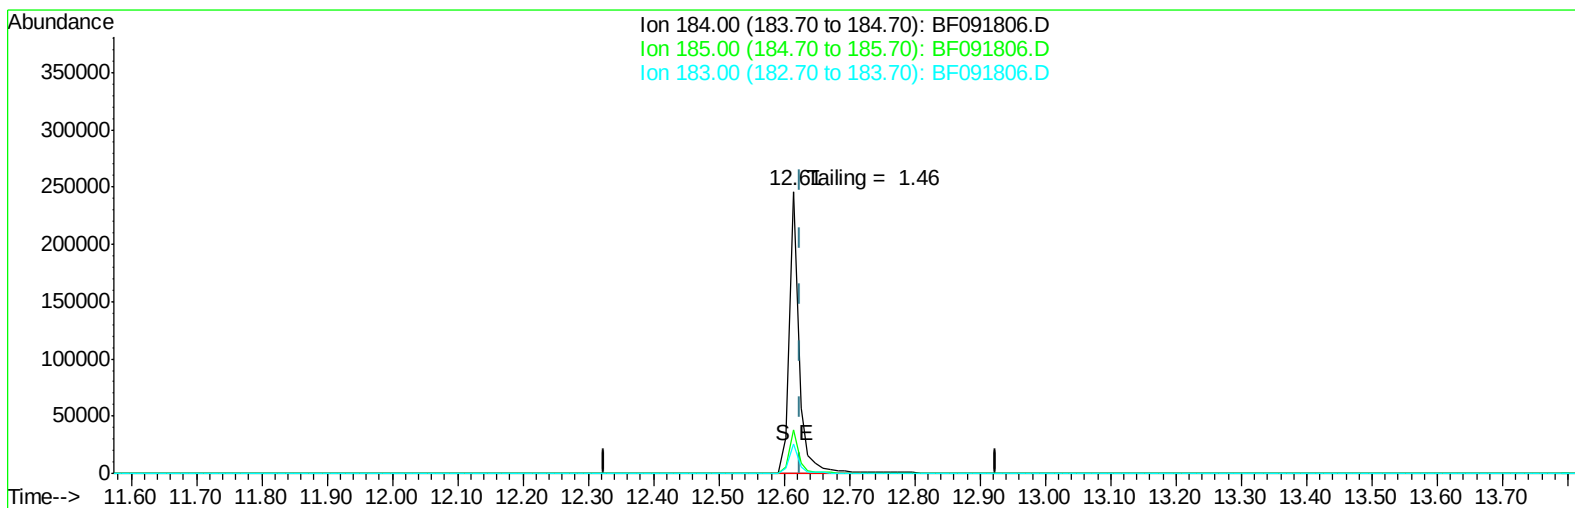

TIC: BF091806.D

(76) Benzidine

12.614min (-0.011) 42013.61ng

response 262434

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.61
183.00	11.50	10.64
0.00	0.00	0.00