


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122016\
 Data File : BF091806.D
 Acq On : 20 Dec 2016 8:20
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 17 22:53:54 2016

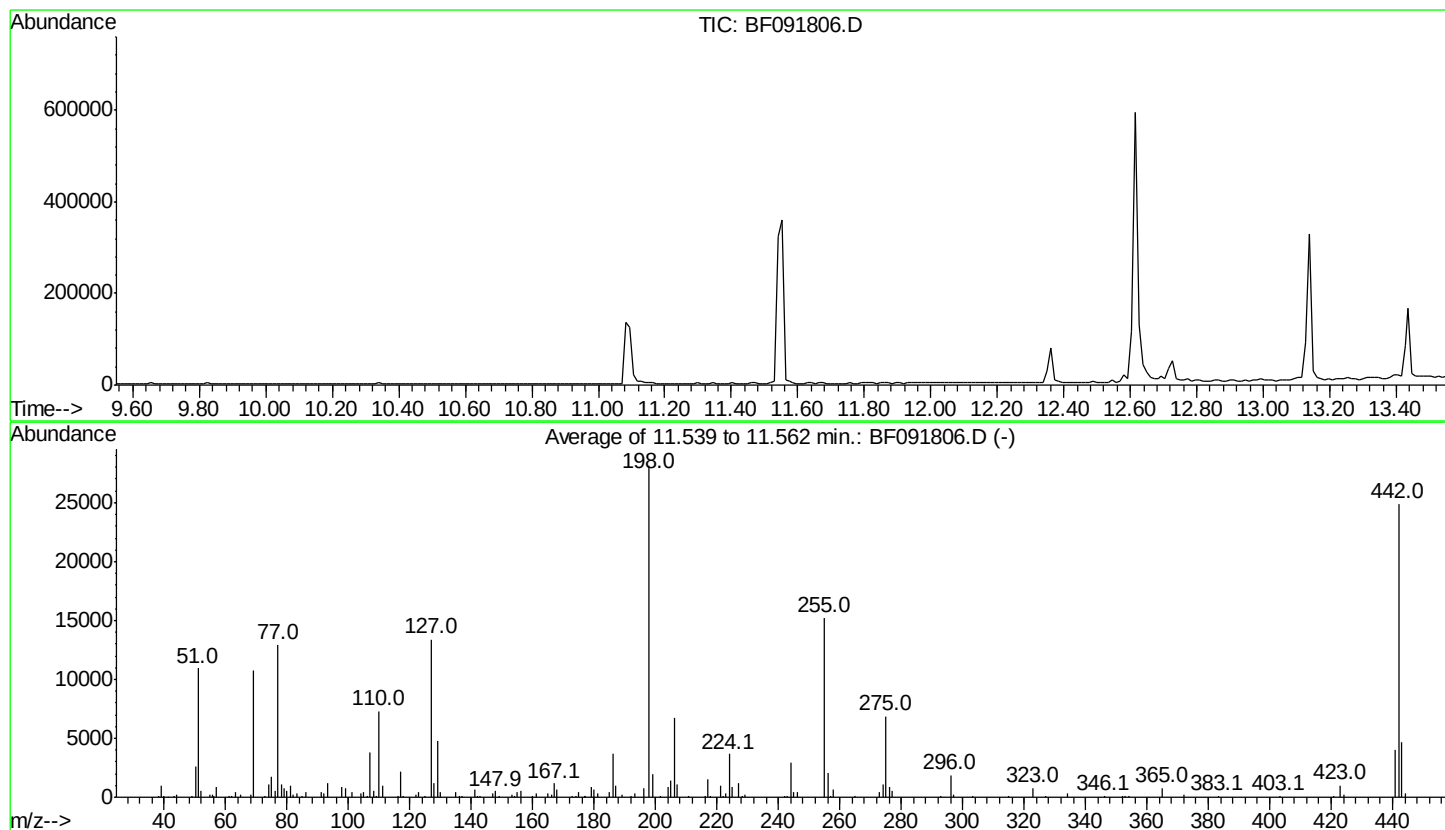

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	10958	PASS
68	69	0.00	2	1.8	193	PASS
69	198	0.00	100	38.1	10710	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.6	13389	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28142	PASS
199	198	5	9	6.9	1934	PASS
275	198	10	60	24.4	6865	PASS
365	198	1	100	2.8	791	PASS
441	442	0.01	24	16.3	4063	PASS
442	198	50	100	88.4	24887	PASS
443	442	15	24	18.7	4650	PASS