
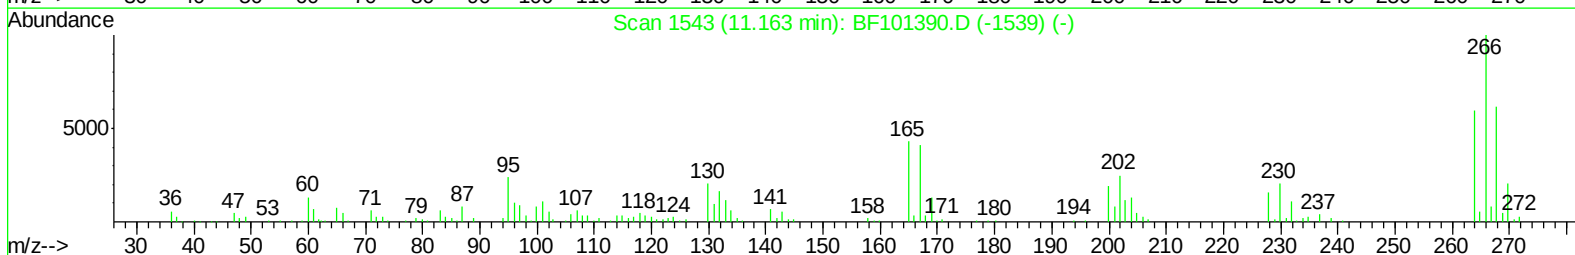
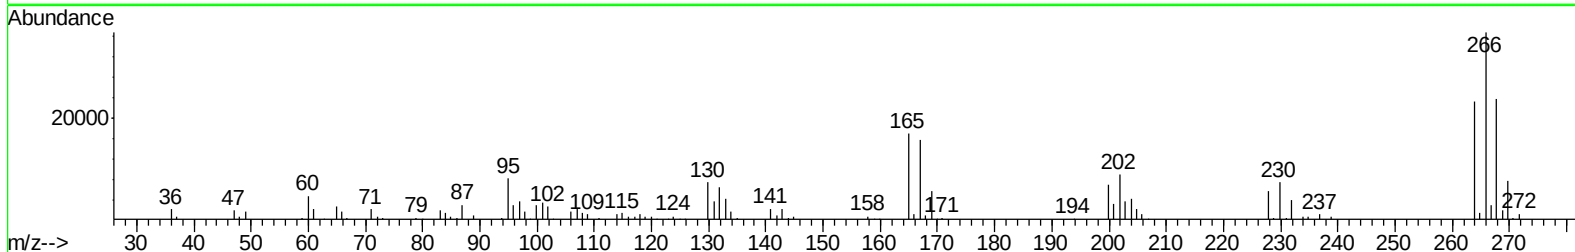


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122017\
Data File : BF101559.D
Acq On : 20 Dec 2017 10:50
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 11:40:56 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 20 14:25:04 2017
Response via : Initial Calibration

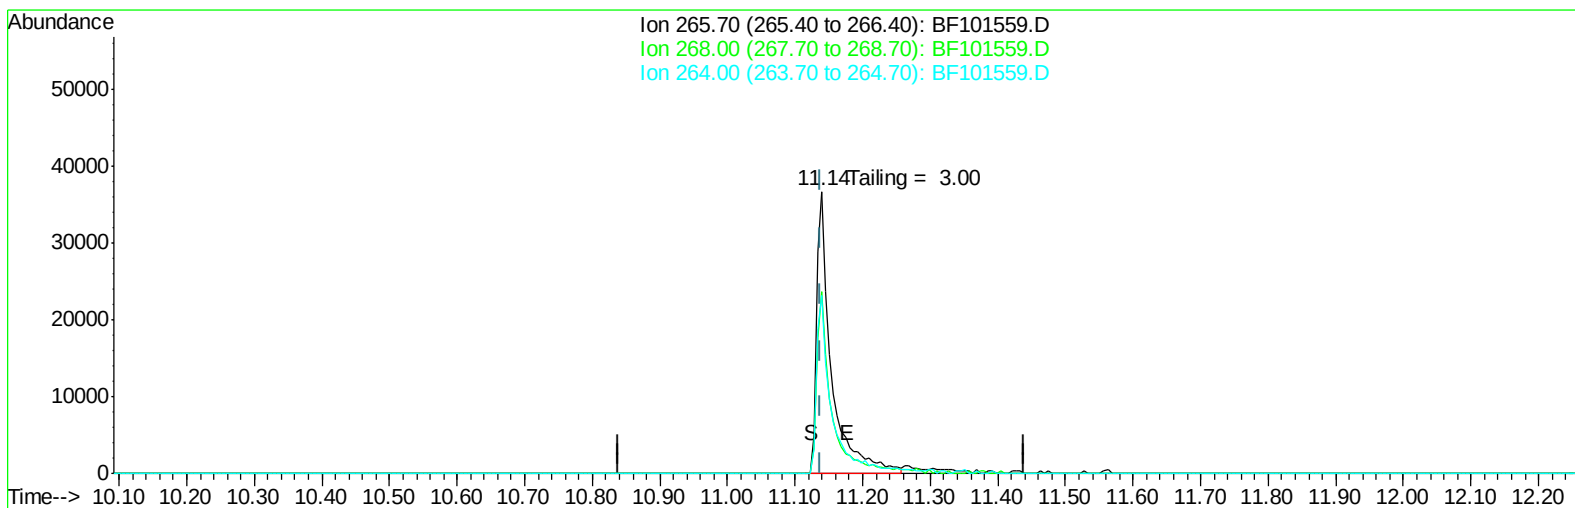

TIC: BF101559.D

(69) Pentachlorophenol (C)




11.139min (-0.000) 31121.44ng

response 57053

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.61
264.00	61.90	63.22
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122017\
 Data File : BF101559.D
 Acq On : 20 Dec 2017 10:50
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 11:40:56 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 20 14:25:04 2017
 Response via : Initial Calibration

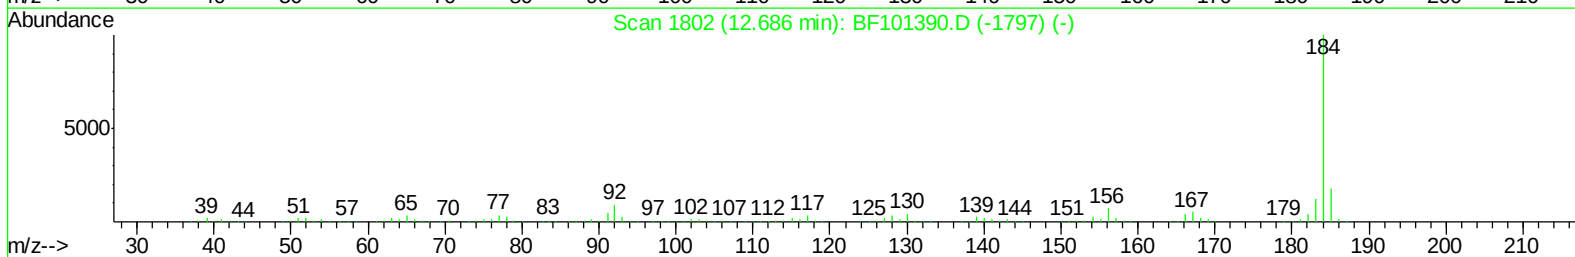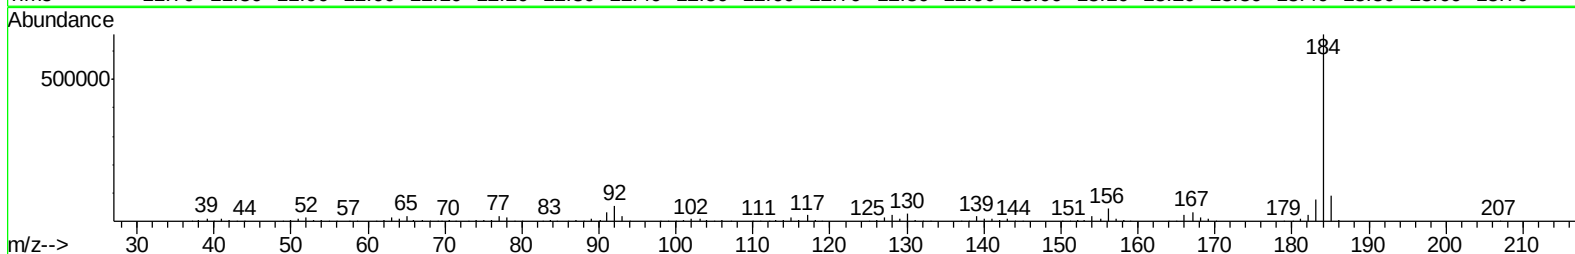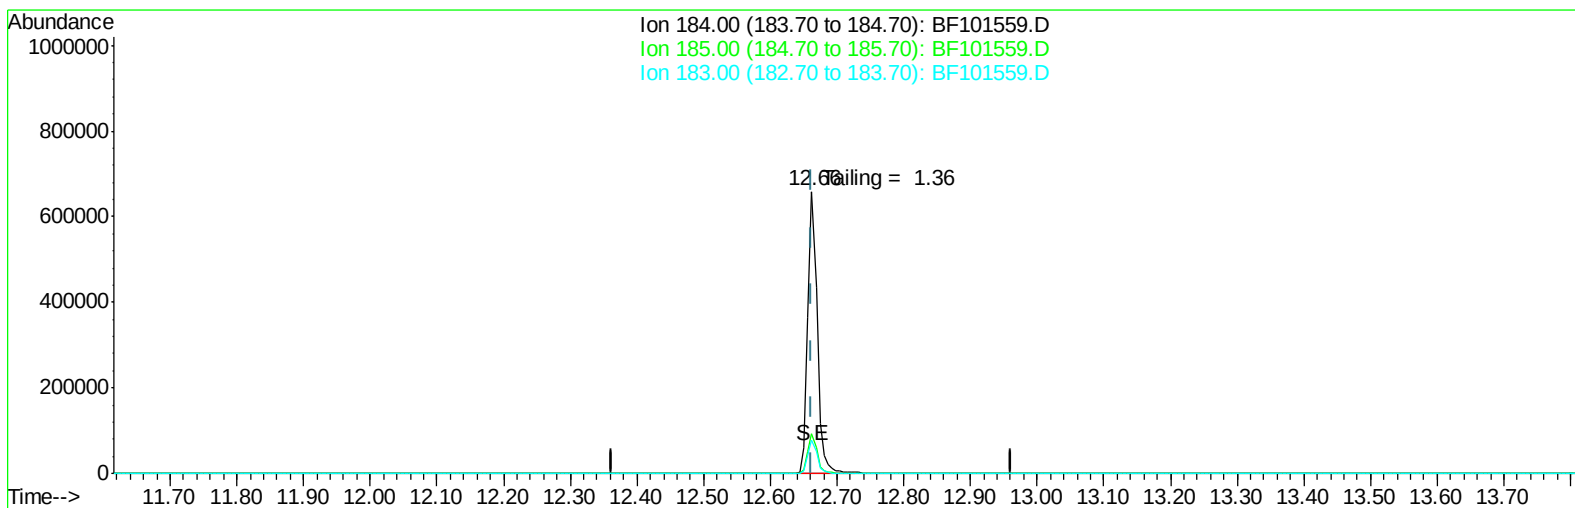

TIC: BF101559.D

(76) Benzidine

12.663min (-0.000) 0.00ng

response 619161

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.01
183.00	11.60	11.98
0.00	0.00	0.00