
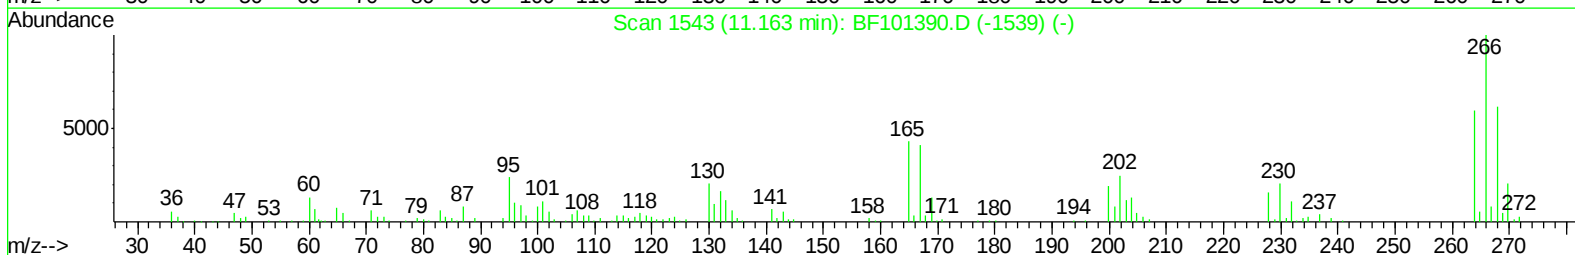
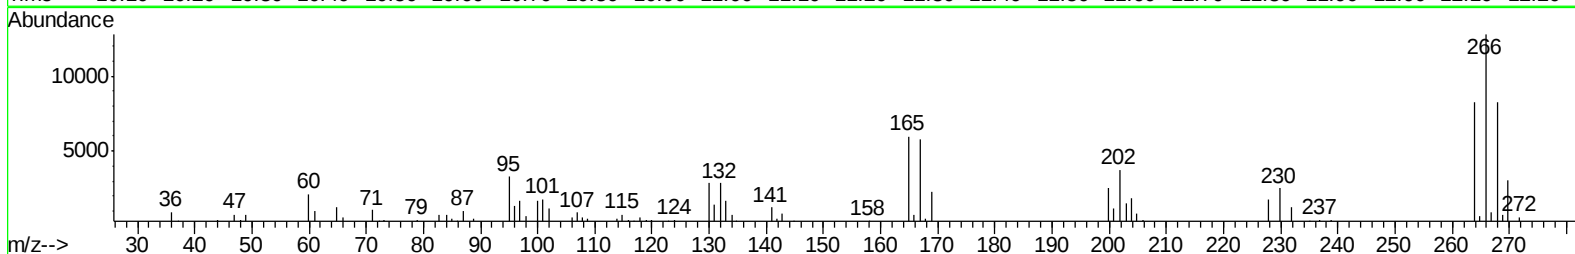


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122017\
Data File : BF101585.D
Acq On : 21 Dec 2017 00:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 11:43:15 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 20 14:25:04 2017
Response via : Initial Calibration

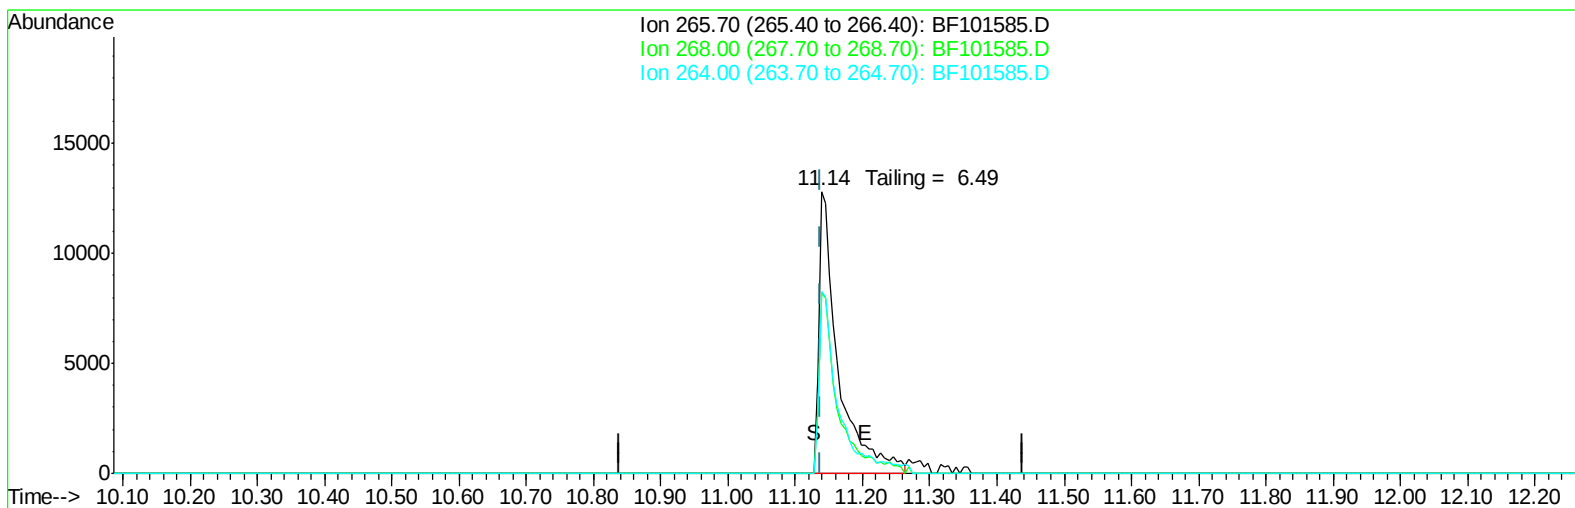

TIC: BF101585.D

(69) Pentachlorophenol (C)




11.139min (-0.000) 44061.25ng

response 25743

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.29
264.00	61.90	64.73
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122017\
Data File : BF101585.D
Acq On : 21 Dec 2017 00:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 11:43:15 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 20 14:25:04 2017
Response via : Initial Calibration

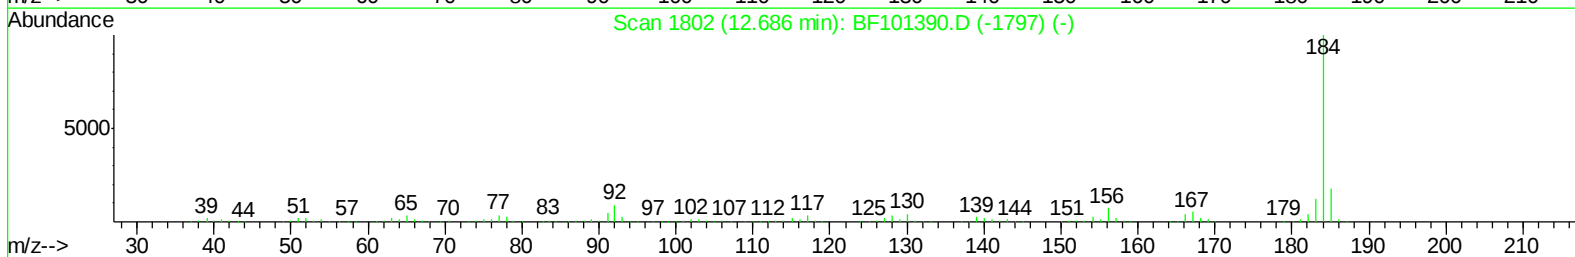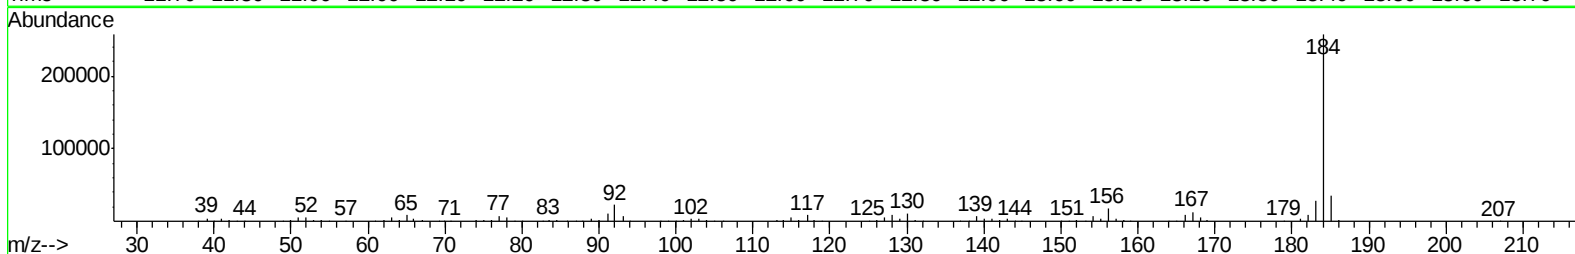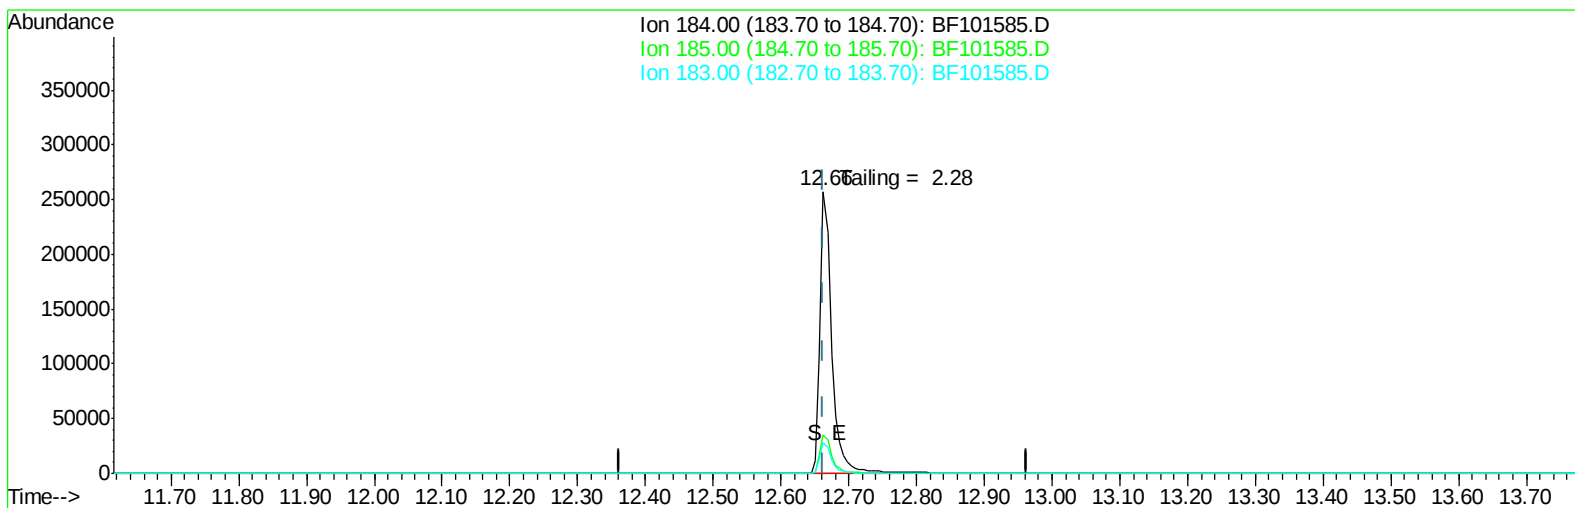

TIC: BF101585.D

(76) Benzidine

12.663min (-0.000) 0.00ng

response 298276

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.75
183.00	11.60	11.15
0.00	0.00	0.00