


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122017\
Data File : BF101559.D
Acq On : 20 Dec 2017 10:50
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 20 14:25:04 2017

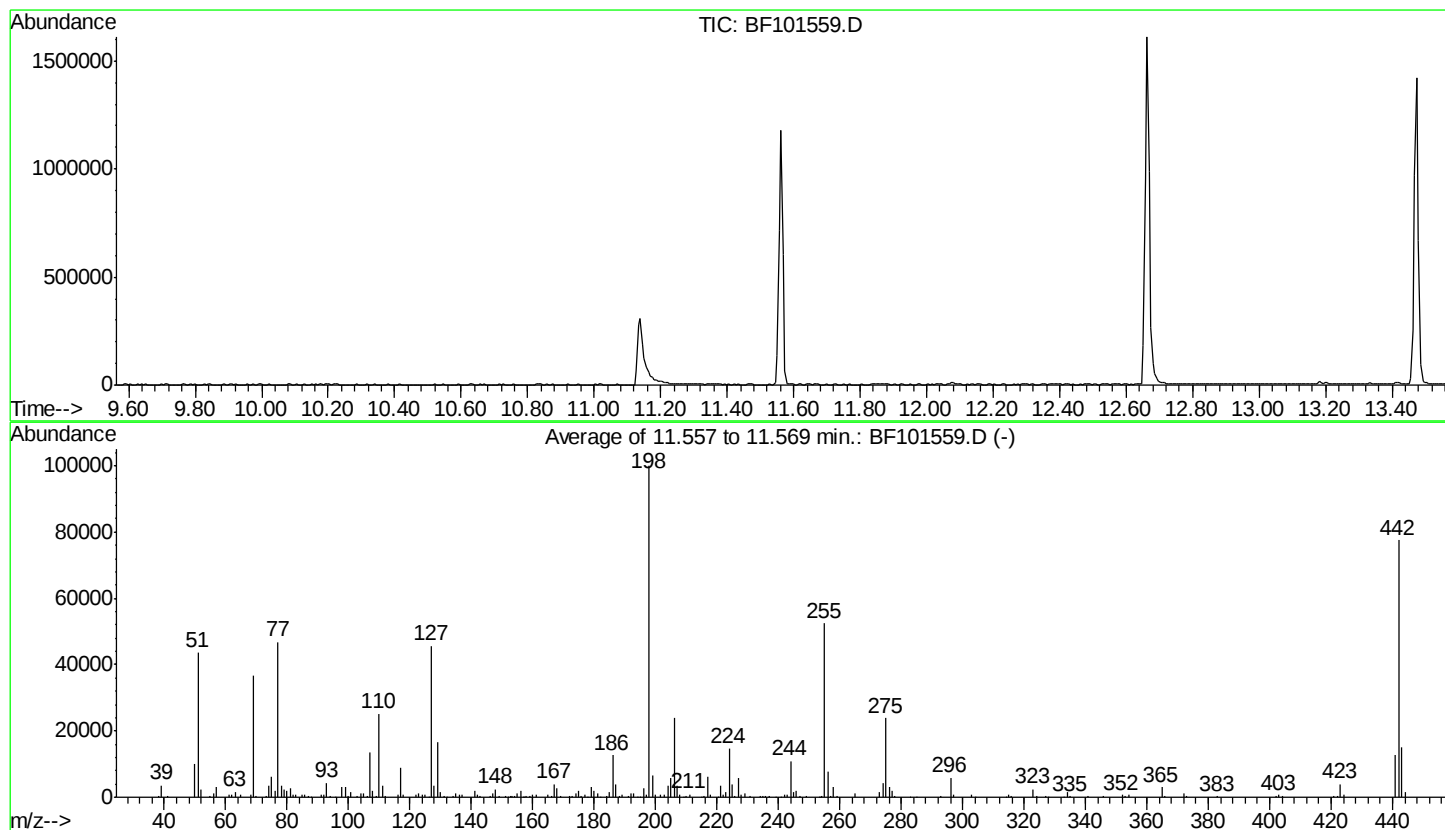

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	43484	PASS
68	69	0.00	2	1.7	625	PASS
69	198	0.00	100	36.8	36826	PASS
70	69	0.00	2	0.6	220	PASS
127	198	10	80	45.7	45688	PASS
197	198	0.00	2	0.9	941	PASS
198	198	100	100	100.0	100032	PASS
199	198	5	9	6.6	6597	PASS
275	198	10	60	23.8	23834	PASS
365	198	1	100	2.9	2920	PASS
441	443	0.01	100	84.2	12597	PASS
442	198	50	100	77.5	77528	PASS
443	442	15	24	19.3	14955	PASS