


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122017\
 Data File : BF101585.D
 Acq On : 21 Dec 2017 00:01
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 20 14:25:04 2017

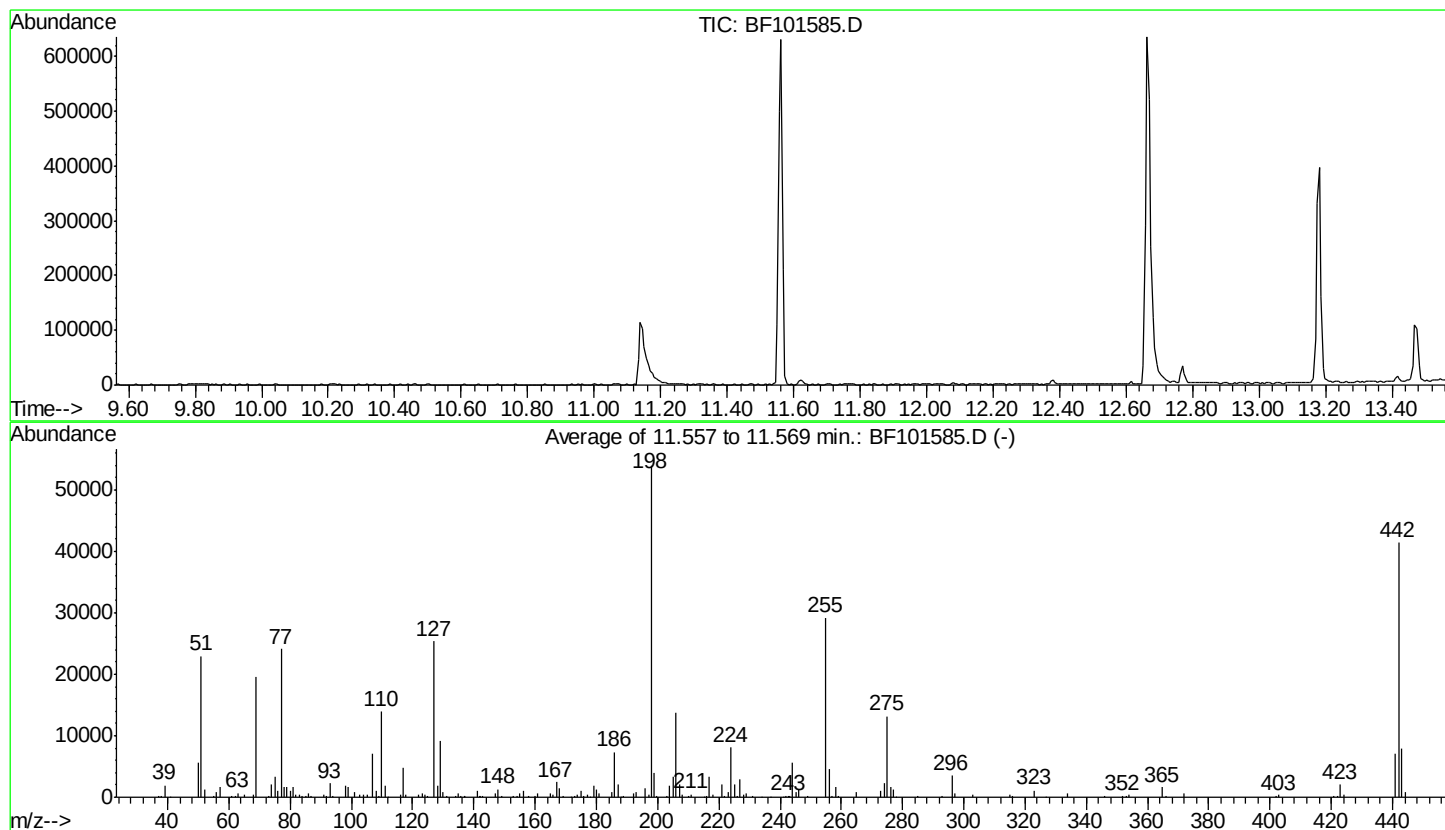

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	22969	PASS
68	69	0.00	2	2.0	400	PASS
69	198	0.00	100	36.3	19612	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.0	25357	PASS
197	198	0.00	2	0.8	455	PASS
198	198	100	100	100.0	53954	PASS
199	198	5	9	7.2	3907	PASS
275	198	10	60	24.4	13160	PASS
365	198	1	100	3.0	1603	PASS
441	443	0.01	100	90.8	7148	PASS
442	198	50	100	76.7	41408	PASS
443	442	15	24	19.0	7868	PASS