
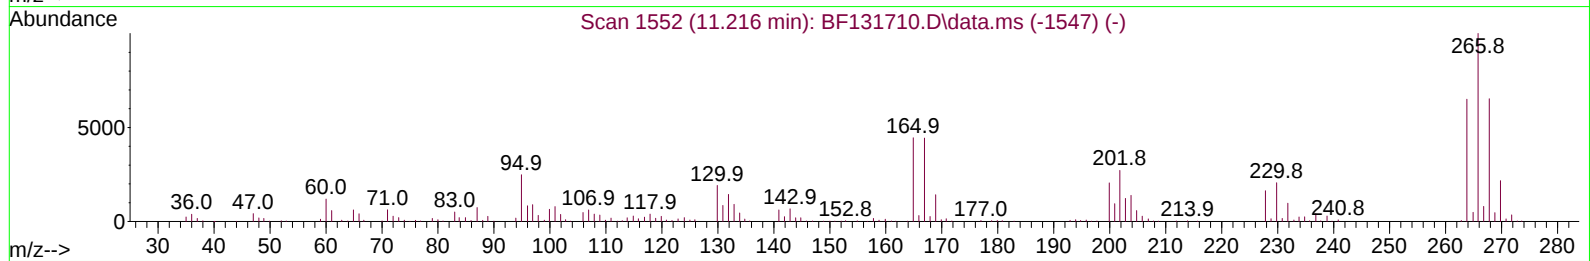
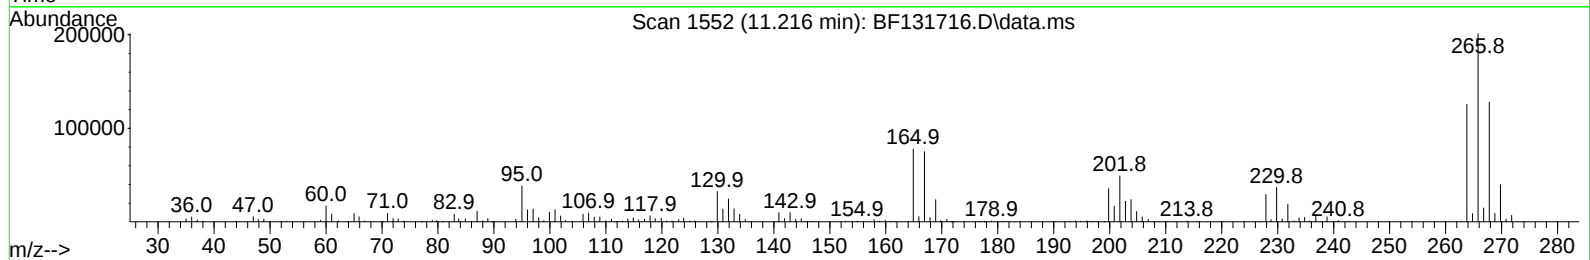


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122022\
 Data File : BF131716.D
 Acq On : 20 Dec 2022 16:48
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 06:27:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 21 03:12:37 2022
 Response via : Initial Calibration

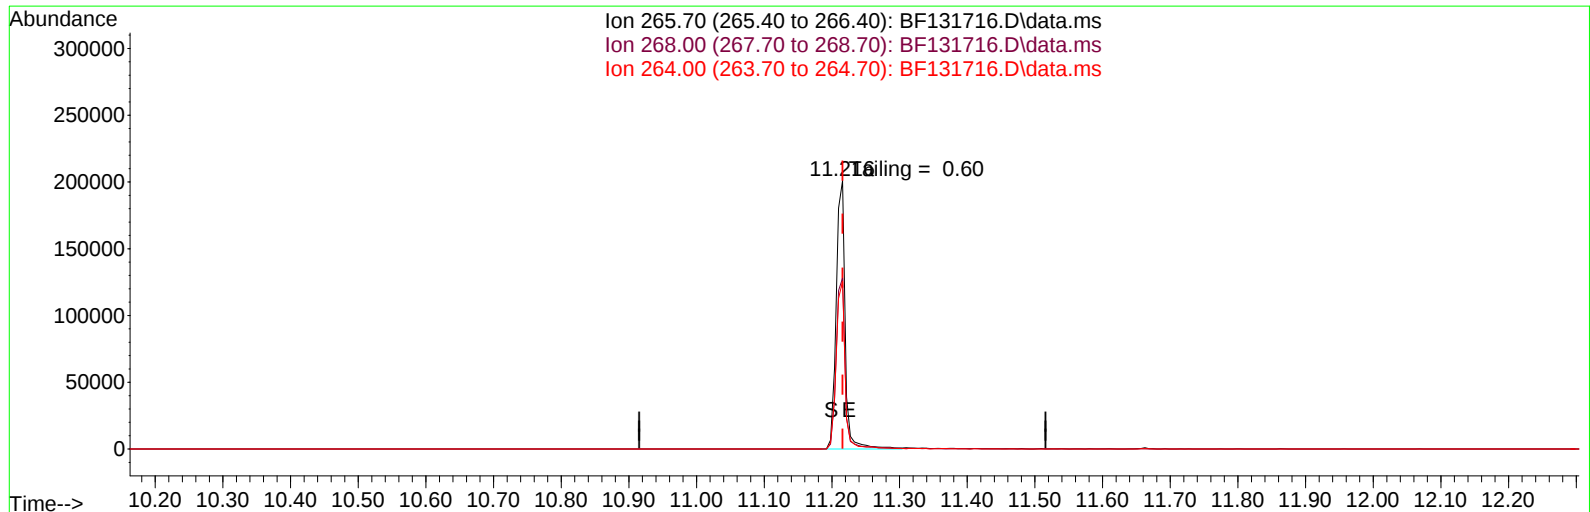

TIC: BF131716.D\data.ms

(70) Pentachlorophenol (C)




11.216min (+ 0.000) 488275.70 ng

response 185146

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.67
264.00	65.00	62.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122022\
 Data File : BF131716.D
 Acq On : 20 Dec 2022 16:48
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 06:27:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 21 03:12:37 2022
 Response via : Initial Calibration

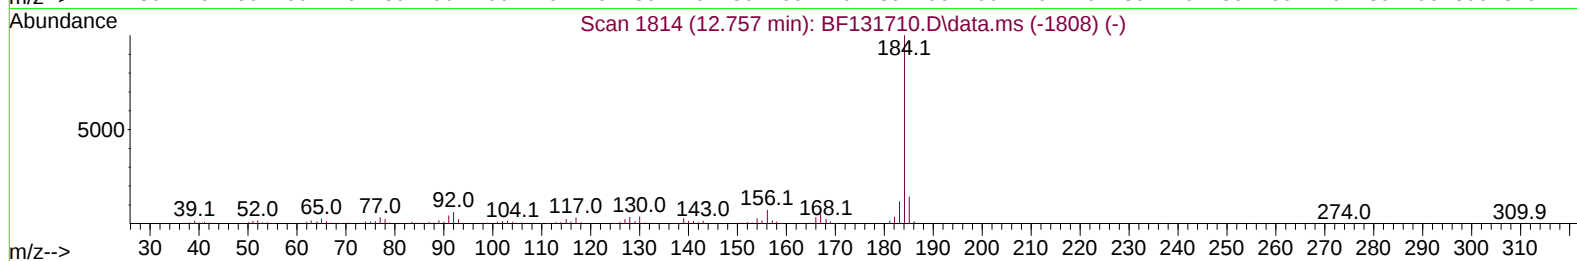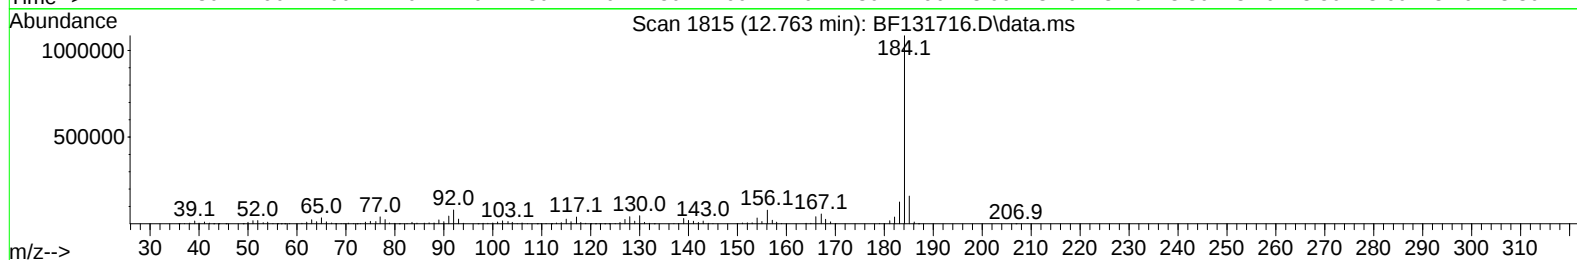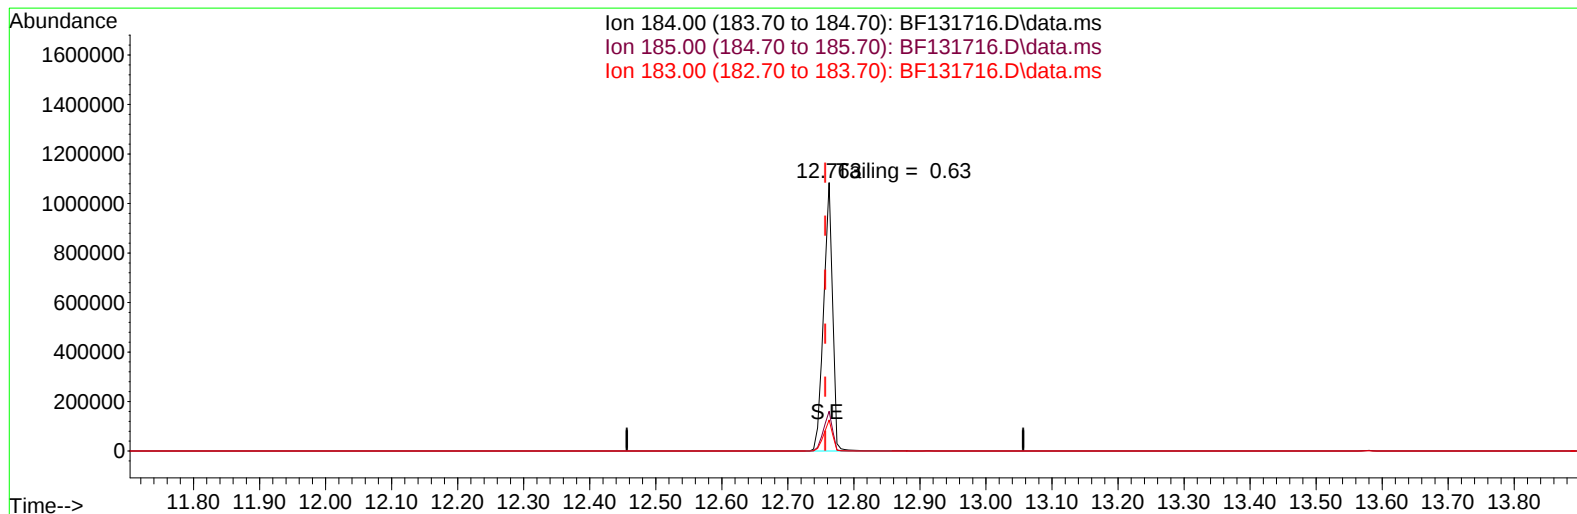

TIC: BF131716.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 0.00 ng

response 1021042

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.77
183.00	11.60	11.58
0.00	0.00	0.00